



Rig Rat III Detector

Wireless Multi-Point Gas Detection System

User Manual



Limited Warranty & Limitation of Liability

BW Technologies LP (BW) warrants this product to be free from defects in material and workmanship under normal use and service for a period of two years, beginning on the date of shipment to the buyer. This warranty extends only to the sale of new and unused products to the original buyer. BW's warranty obligation is limited, at BW's option, to refund of the purchase price, repair, or replacement of a defective product that is returned to a BW authorized service center within the warranty period. In no event shall BW's liability hereunder exceed the purchase price actually paid by the buyer for the Product.

This warranty does not include:

- a) fuses, disposable batteries or the routine replacement of parts due to the normal wear and tear of the product arising from use;
- b) any product which in BW's opinion, has been misused, altered, neglected or damaged by accident or abnormal conditions of operation, handling or use;
- c) any damage or defects attributable to repair of the product by any person other than an authorized dealer, or the installation of unapproved parts on the product; or

The obligations set forth in this warranty are conditional on:

- a) proper storage, installation, calibration, use, maintenance and compliance with the product manual instructions and any other applicable recommendations of BW;
- b) the buyer promptly notifying BW of any defect and, if required, promptly making the product available for correction. No goods shall be returned to BW until receipt by the buyer of shipping instructions from BW; and
- c) the right of BW to require that the buyer provide proof of purchase such as the original invoice, bill of sale or packing slip to establish that the product is within the warranty period.

THE BUYER AGREES THAT THIS WARRANTY IS THE BUYER'S SOLE AND EXCLUSIVE REMEDY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. BW SHALL NOT BE LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL OR CONSEQUENTIAL DAMAGES OR LOSSES, INCLUDING LOSS OF DATA, WHETHER ARISING FROM BREACH OF WARRANTY OR BASED ON CONTRACT, TORT OR RELIANCE OR ANY OTHER THEORY.

Since some countries or states do not allow limitation of the term of an implied warranty, or exclusion or limitation of incidental or consequential damages, the limitations and exclusions of this warranty may not apply to every buyer. If any provision of this warranty is held invalid or unenforceable by a court of competent jurisdiction, such holding will not affect the validity or enforceability of any other provision.

Canada

BW Technologies LP
2840 – 2nd Avenue SE
Calgary, AB
Canada T2A 7X9

USA

BW America
3279 West Pioneer Parkway
Arlington, TX
USA 76013

Europe

BW Europe
5 Canada Close
Banbury, Oxfordshire
United Kingdom OX16 2RT

Table of Contents

Title	Page
Introduction.....	1
Contacting BW Technologies.....	3
Safety Information - Read First	3
Getting Started	7
Rig Rat III Detector.....	8
External Components	8
Operations Bay Panel.....	9
Internal Components	10
Display Elements	11
Main System Components and Option Devices.....	12
Detector Pushbuttons	13
Detector Mounting Requirements.....	14
Installation	15
Installation Location	15
The Detector	15
The Antenna	16
Mounting the Detector	17
Cable Installation	17
Grounding the Detector	17
Setting the Detector and Transceiver Channels.....	20
The Sensors.....	22
Sensor Locations	22
Sensor Installation	23
Sensor Measuring Ranges	25
Installing Optional Devices/Accessories	26
Independent Power	26

Battery Life	27
Battery Level	28
Line Power	28
Charger Power	28
Applying Power	28
Sensor Readout Status	29
Calibration and Setting Alarm Setpoints	29
Guidelines	30
When to Calibrate	30
Calibration Features	30
Setting the Alarm Setpoints	32
Calibrating Stainless Steel Sensors	33
Calibrating Encapsulated Sensors	33
Transmission Interval	36
End Calibration	38
Alarms	39
Viewing the Maximum Gas Level	43
Setting Dipswitches for Alarm Options	43
Alarm Option Features and Exceptions	45
Maintenance	45
Replacing the Fuse (500mA)	46
Storage and Transport	46
Prior to Storage or Transport	46
System Test	48
Test Signal Transmission and Reception	48
Test Sensor Integrity Alarm	48
Test Low and High Alarm Functions	49
System Inspection	49
Troubleshooting	50
Replacement Parts and Accessories	52
Specifications	54
Appendix A Encapsulated Sensors	57

Sensor Specifications (Encapsulated).....	58
Calibration Gas Specifications.....	61
Measuring Ranges for Encapsulated Sensors.....	62
Relative Sensitivity of Combustible Gases/Vapours	63
Appendix B Installation Requirements.....	65
Installation of an Unapproved Charger — Detector	66
Installation of an Unapproved External Charger	68
IS Sensor Barrier Installation.....	74
Appendix C Stainless Steel Sensors	75
Stainless Steel Sensors (Toxic/O ₂)	76
Calibration (Stainless Steel Sensors).....	76
Transmission Interval.....	78
End Calibration	80
Maintenance	80
Specifications (Stainless Steel Sensors).....	82
Measuring Ranges for Stainless Steel Sensors	86

List of Tables

Table	Title	Page
1.	The Rig Rat III Detector	2
2.	Gases Monitored	2
3.	International Symbols	6
4.	Rig Rat III External Components	8
5.	Operations Bay Panel.....	9
6.	Detector Internal Components.....	10
7.	Display Elements	11
8.	Main System Components.....	12
9.	Pushbuttons.....	13
10.	System Cable Connection	17
11.	Sensor Measuring Range Selection	26
12.	Sensor Types and Battery Life	27
13.	Sensor Stabilization	29
14.	Default Factory Settings	31
15.	Alarms.....	39
16.	Default Alarm Dip Switch Settings.....	44
17.	Alarm Dip Switch Settings	44
18.	Troubleshooting Tips	50
19.	Replacement Parts and Accessories	52
20.	Operating and Calibration Specifications for Each Encapsulated Sensor	58
21.	Encapsulated Sensor Measuring Ranges	62
22.	Relative Sensitivity of Combustible Gases/Vapours	63
23.	Limiting Energy	67
24.	I.S. Barrier Example.....	70
25.	I.S. Barrier Configurations	73

26.	I.S. Barrier Requirements	73
27.	Toxic/O ₂ Sensor Replacement Parts	81
28.	Operating and Calibration Specifications for Each Stainless Steel Sensor	83
29.	Stainless Steel Sensor Measuring Ranges	86

List of Figures

Figure	Title	Page
1.	Rig Rat III External Components	8
2.	Operations Bay Panel.....	9
3.	Detector Internal Components.....	10
4.	Display Elements	11
5.	Main System Components.....	12
6.	Mounting Requirements	14
7.	Confined Space Installation	15
8.	Bonding the Detector	18
9.	Bonding with Bonding Cable	19
10.	Grounding Rod Installation	20
11.	RIG RAT III Transceiver	21
12.	Channel Rotary Switch	21
13.	Transceiver A and B Channels	21
14.	Sensor Ports on Detector	23
15.	Sensor Dimensions (Encapsulated)	24
16.	Labeling the Sensors on the Detector	24
17.	Sensor Measuring Range Rotary Switches.....	25
18.	Battery Levels	28
21.	Sensor Magnet and Magnetic Pen	33
19.	Calibrating the Encapsulated Sensor	34
20.	Calibration Connections	35
22.	Measuring Range Dip Switches	43
23.	Pin A and Pin B Option Ports	45
24.	Gas Detection System Interconnection	66
25.	Division 2 Unapproved External Charger Installation.....	68
26.	Division 1 Unapproved External Charger Installation.....	69
27.	Division 2 Unapproved Accessory Installation	71

28.	Division 1 Unapproved Accessory Installation	72
29.	Approved IS Sensor Barrier Installation	74
30.	Sensor Dimensions (Stainless Steel)	76
31.	Cylinder Connection for Calibration	77
32.	Calibration Cap and Blanking Plugs	80
33.	Toxic/O ₂ Sensor Replacement	81

Rig Rat III Detector

Introduction

Warning

To ensure your personal safety, read the [Safety Information](#) before using the detector.

The Rig Rat III Detector (the detector) is a wireless* multi-point gas detection system that emits an alarm when hazardous gas levels exceed the user-selectable alarm setpoints.

**Model RR-3000S is a non-wireless multi-point gas detection system. All reference to wireless transmission, antennas, and transceivers does not apply to this model.*

The detector is an area safety device. It is your responsibility to respond properly to the alarm.

Refer to Table 2 for the gases that are monitored by the Rig Rat III detector.

CAUTION: FOR SAFETY REASONS, THIS EQUIPMENT MUST BE OPERATED AND SERVICED BY QUALIFIED PERSONNEL ONLY. READ AND UNDERSTAND THE USER MANUAL COMPLETELY BEFORE OPERATING OR SERVICING.

Table 1. The Rig Rat III Detector

Order Number	Description
RR-3000	Wireless multi-point gas detection system
RR-3000S	Non-wireless multi-point gas detection system

Table 2. Gases Monitored

Gas Detected	Unit of Measure
H ₂ S (Hydrogen sulfide)	parts per million (ppm)
CO (Carbon monoxide)	parts per million (ppm)
O ₂ (Oxygen)	percent by volume (%)
LEL (Combustibles)	percent of lower explosive limit (% LEL)
SO ₂ (Sulfur dioxide)	parts per million (ppm)
NH ₃ (Ammonia)	parts per million (ppm)
Cl ₂ (Chlorine)	parts per million (ppm)
H ₂ (Hydrogen)	parts per million (ppm)
HCN (Hydrogen cyanide)	parts per million (ppm)
HCL (Hydrogen chloride)	parts per million (ppm)
NO ₂ (Nitrogen dioxide)	parts per million (ppm)
CLO ₂ (Chlorine dioxide)	parts per million (ppm)
C ₂ H ₅ OH (Ethanol)	parts per million (ppm)
C ₂ H ₄ O (Ethylene oxide)	parts per million (ppm)
NO (Nitric oxide)	parts per million (ppm)
O ₃ (Ozone)	parts per million (ppm)
PH ₃ (Phosphine)	parts per million (ppm)

Contacting BW Technologies

To contact BW Technologies call:

USA: 1-888-749-8878

Canada: 1-800-663-4164

Europe: +44 (0) 1295 700300

Anywhere in the world: +1-403-248-9226

Address correspondence to:

BW Technologies LP
2840 – 2 Avenue S.E.
Calgary, AB T2A 7X9
CANADA

Email us at: info@bwt.net

Visit BW Technologies' web site at: www.gasmonitors.com

ISO 9001

Safety Information - Read First

Use the detector only as specified in this manual, otherwise the protection provided by the instrument may be impaired.

International symbols used on the detector and in this manual are explained in Table 3.

Read the **Warnings** and **Cautions** on the following pages before using the detector.



Note

This instrument contains batteries. Do not mix with the solid waste stream. Spent batteries should be disposed of by a qualified recycler or hazardous materials handler.

⚠ Cautions

- ⇒ **Warning: Substitution of components may impair Intrinsic Safety.**
- ⇒ **Do not use the detector if it or any system components are damaged. Inspect the system on a regular basis and maintain a record log.**
- ⇒ **If the detector is damaged or parts are missing, contact [BW Technologies](#) immediately.**
- ⇒ **To prevent ignition of a flammable or combustible atmosphere, disconnect the power before servicing.**
- ⇒ **To prevent damage to fuses and internal components of the detector, disconnect the power before servicing.**
- ⇒ **When installing cables, ensure they are protected from possible damage. Secure the cables in place and fasten any excess. Do not exceed a 65° bend allowance when installing the cables.**
- ⇒ **Ensure that all plug-in connectors are clean and fully seated when installing.**
- ⇒ **Ensure that the weatherproof ring on the connector(s) is fully screwed down.**
- ⇒ **Ensure all ports that are not in use are completely screwed down and the port cover caps are installed.**
- ⇒ **Ensure the latch on the external hinged door is securely connected and that the handle has been turned the full 180° to complete the weather seal.**
- ⇒ **Do not expose the detector to electrical shock and/or severe mechanical shock.**
- ⇒ **Do not install the detector in an atmosphere that contains ketones, alcohols, or acids.**
- ⇒ **Use only sensors that are specifically designed for the Rig Rat III system. Refer to [Encapsulated Sensor Measuring Ranges](#), [Stainless Steel Sensor Measuring Ranges](#), and/or [Replacement Parts and Accessories](#).**


⚠ Cautions

- ⇒ **Ensure the sensor screen is not blocked.**
- ⇒ **Calibrate the detector before first-time use and continue on a regular schedule, depending upon use and sensor exposure to poisons and contaminants. BW recommends calibration minimum once every 90 days (3 months).**
- ⇒ **BW recommends that a bump check be performed before each day's use to verify correct instrument operation. Calibrate if the readings are not within the specified limits.**
- ⇒ **Periodically bump check each sensor to confirm accurate response to gas. Expose the detector to a targeted gas concentration that exceeds the high alarm setpoints, and manually verify that the audible and visual alarms are activated.**
- ⇒ **BW recommends that the combustible sensor be checked with a known concentration of calibration gas after any known exposure to contaminants/poisons (e.g., sulfur compounds, silicon vapors, halogenated compounds, etc.).**
- ⇒ **Protect the combustible sensor from exposure to lead compounds, silicones, butane from a cigarette lighter, and chlorinated hydrocarbons. Although certain organic vapors (such as, leaded gasoline and halogenated hydrocarbons) may temporarily inhibit sensor performance, in most cases the sensor will recover after calibration.**
- ⇒ **Any rapid up-scaling reading, followed by a declining or erratic reading, may indicate a gas concentration beyond upper scale limit that may be hazardous.**
- ⇒ **The combustible sensor is factory calibrated to 50% LEL methane. If monitoring a different combustible gas in the % LEL range, calibrate the sensor using the appropriate gas. High off-scale % LEL of % v/v methane readings may indicate an explosive concentration.**

⚠ Cautions

- ⇒ Extended exposure of the detector's sensors to specific concentrations of combustible gases and air may stress a detector element that can seriously affect performance. If an alarm occurs due to high concentrations of combustible gases, recalibration should be performed, or if required, replace the sensor.
- ⇒ Do not allow liquids to condense or use high power sprays on the instruments. Do not attach/connect system components that do not meet specified criteria, such as alarms, relays, cabling, etc.
- ⇒ Do not attempt to disassemble, adjust, or service the detector unless instructions for that procedure are specified in the user manual and/or that part is listed as a replacement part. Use only BW Technologies [Replacement Parts and Accessories](#).
- ⇒ The detector warranty is void if customer, personnel, or third parties damage the detector during repair attempts. Non-BW Technologies repair/service attempts void this warranty. Use only sensors that are specifically designed for the Rig Rat III system. Refer to [Encapsulated Sensor Measuring Ranges](#), [Stainless Steel Sensor Measuring Ranges](#), and [Replacement Parts and Accessories](#).

Table 3. International Symbols

Symbol	Meaning
	Approved to both U.S. and Canadian Standards by the Canadian Standards Association.

Getting Started

The items listed below are included with the detector. If the detector is damaged or parts are missing, contact the place of purchase immediately.

- 5 dBi antenna
- Security key
- Phillips screwdriver
- Slot-regular screwdriver
- Rig Rat III Wireless Multi-Point Gas Detection User Manual

To order replacement parts, refer to [Replacement Parts and Accessories](#).

To become familiar with the features and functions of the detector, refer to the following figures and tables:

- Figure 1 and Table 4 describe the main external components of the detector.
- Figure 2 and Table 5 describe the operation bay panel of the detector.
- Figure 3 and Table 6 describe the internal components of the detector.
- Figure 4 and Table 7 describe the liquid crystal display (LCD) elements of the detector.
- Figure 5 and Table 8 describe the main system components and the option devices of the detector.
- Table 9 describes the detector pushbuttons and functions.

Rig Rat III Detector

The Rig Rat III detector (“the detector”) is a fixed gas detection unit that can be used independently or operate in conjunction with the Rig Rat III Controller (“the controller”).

External Components

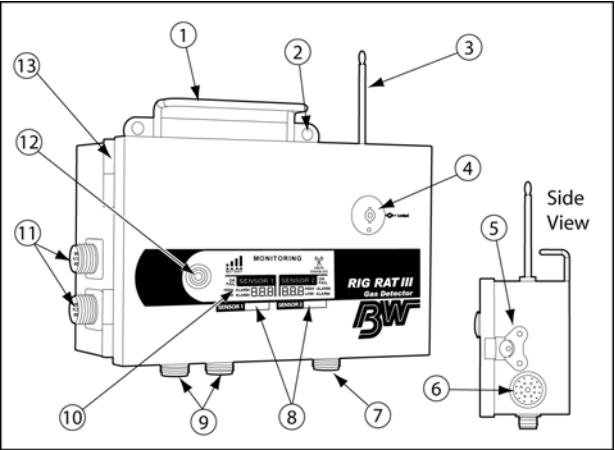


Figure 1. Rig Rat III External Components

Table 4. Rig Rat III External Components

Item	Description
1	Carrying handle
2	Mounting bracket
3	TNC antenna
4	Security key
5	External tension latch
6	Audible alarm
7	CHARGER PORT
8	Gas label bars
9	OPTION PORTS (two)
10	Liquid crystal display (LCD)
11	SENSOR PORTS (two)
12	Red LED alarm
13	External hinged door

Note

If the detector is used with a controller, the detector must be equipped with a transceiver.

Operations Bay Panel

The operations bay panel is designed to provide easy access for activating/deactivating, setting high/low alarm setpoints, enabling/disabling the XMTR, and testing the XMTR.

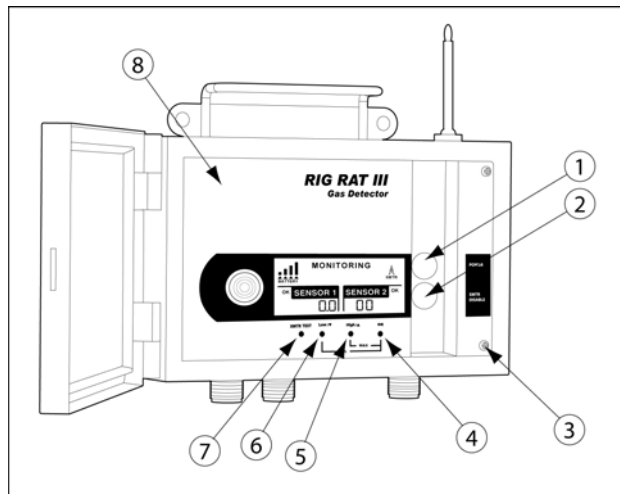


Figure 2. Operations Bay Panel

Table 5. Operations Bay Panel

Item	Description
1	Pushbutton (POWER)
2	Transmitter pushbutton (XMTR DISABLE)
3	Phillips screws (2)
4	Pushbutton (OK)
5	Alarm setpoint/decrement value pushbutton (HIGH / ▲)
6	Alarm setpoint/increment value pushbutton (LOW / ▼)
7	Transmitter pushbutton (XMTR TEST)
8	Service bay hinged door

Calibrations and system tests are also performed from the operations bay panel.

Note

Calibrate the detector every 90 days (3 months).

For calibration guidelines and procedures, refer to [Calibration and Setting Alarm Setpoints](#).

Internal Components

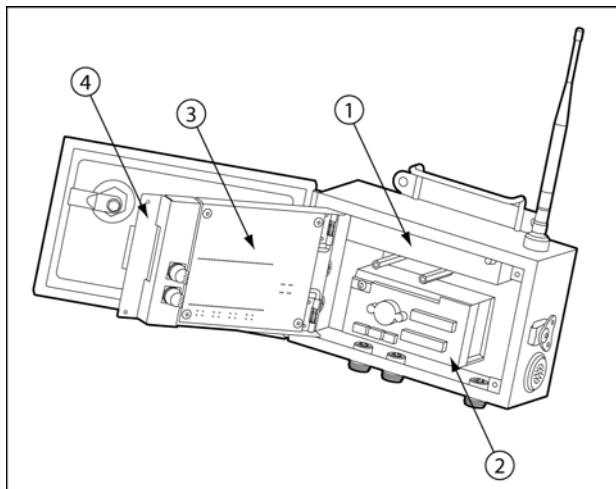


Figure 3. Detector Internal Components

Table 6. Detector Internal Components

Item	Description
1	Transceiver
2	Power board
3	Main board
4	Operations bay panel door

The internal components are used to set the

- sensor types and measuring ranges,
- detector channels,
- transceiver channels, and
- alarm relays for attached option devices.

Display Elements

The liquid crystal display (LCD) provides immediate and detailed information about the sensors, alarm setpoints, and battery life levels.

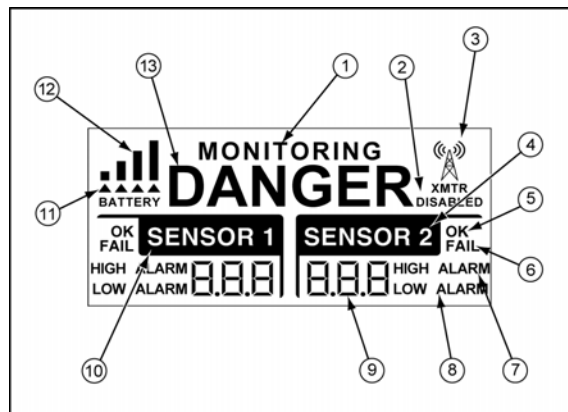


Figure 4. Display Elements

The LCD indicates when it is monitoring, if the XMTR (transmission) is enabled or disabled, and displays information when the detector is in an alarm condition.

Table 7. Display Elements

Item	Description
1	Sensor is MONITORING gas
2	XMTR DISABLED icon
3	XMTR enabled icon
4	SENSOR 2 identifier icon bar
5	Sensor OK
6	Sensor FAIL
7	HIGH ALARM condition
8	LOW ALARM condition
9	Numeric value (ppm or %)
10	SENSOR 1 identifier icon bar
11	BATTERY level indicator
12	Battery level bar graph
13	Flashing DANGER alarm icon

Main System Components and Option Devices

The following figure and table show the exterior connections and available option devices that are used to operate with the detector.

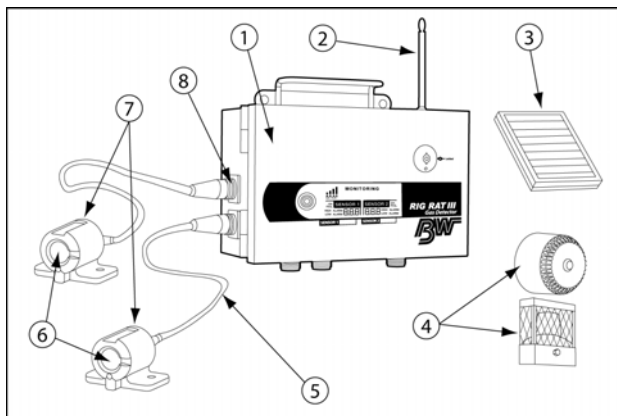


Figure 5. Main System Components

Table 8. Main System Components

Item	Description
1	Rig Rat III
2	5 dBi antenna
3	Trickle and bench chargers (solar or line)
4	Optional remote devices: audible/visual alarms, relays, solenoid driver, etc.
5	Shielded sensor cables
6	Sensor screen(s)
7	Remote sensor(s)
8	Weatherproof ring

Refer to [Installation](#) for procedures and additional information.

Detector Pushbuttons

Table 9. Pushbuttons

Pushbutton	Description
<input type="radio"/> POWER	<ul style="list-style-type: none"> To activate/deactivate the detector, press <input type="radio"/> POWER.
<input type="radio"/> XMTR DISABLE	<ul style="list-style-type: none"> To enable/disable communication between the detector and the controller, press <input type="radio"/> XMTR DISABLE. <p>Note: If the detector is operating with a controller, it must be equipped with a transceiver.</p>
<input type="radio"/> HIGH / ▲	<ul style="list-style-type: none"> To view the high alarm setpoint, press and hold <input type="radio"/> HIGH / ▲. To increment the displayed value (high or low setpoint), press <input type="radio"/> HIGH / ▲. To view the maximum gas level detected by the sensor, press and hold <input type="radio"/> HIGH / ▲ and <input type="radio"/> OK simultaneously for 1 second. To clear the maximum gas level detected, press and hold <input type="radio"/> HIGH / ▲ and <input type="radio"/> OK simultaneously (5 seconds) until CLr displays on the LCD.
<input type="radio"/> LOW / ▼	<ul style="list-style-type: none"> To view the low alarm setpoint, press and hold <input type="radio"/> LOW / ▼. To decrement the displayed value (high or low setpoint), press <input type="radio"/> LOW / ▼. To initiate calibration, press and hold <input type="radio"/> LOW / ▼ and <input type="radio"/> OK simultaneously for 1 second.
<input type="radio"/> OK	<ul style="list-style-type: none"> To accept a selected value, press <input type="radio"/> OK.
<input type="radio"/> XMTR TEST	<ul style="list-style-type: none"> To transmit a countdown sequence to the controller, press <input type="radio"/> XMTR TEST. <p>Note: If the detector is operating with a controller, it must be equipped with a transceiver.</p>

Detector Mounting Requirements

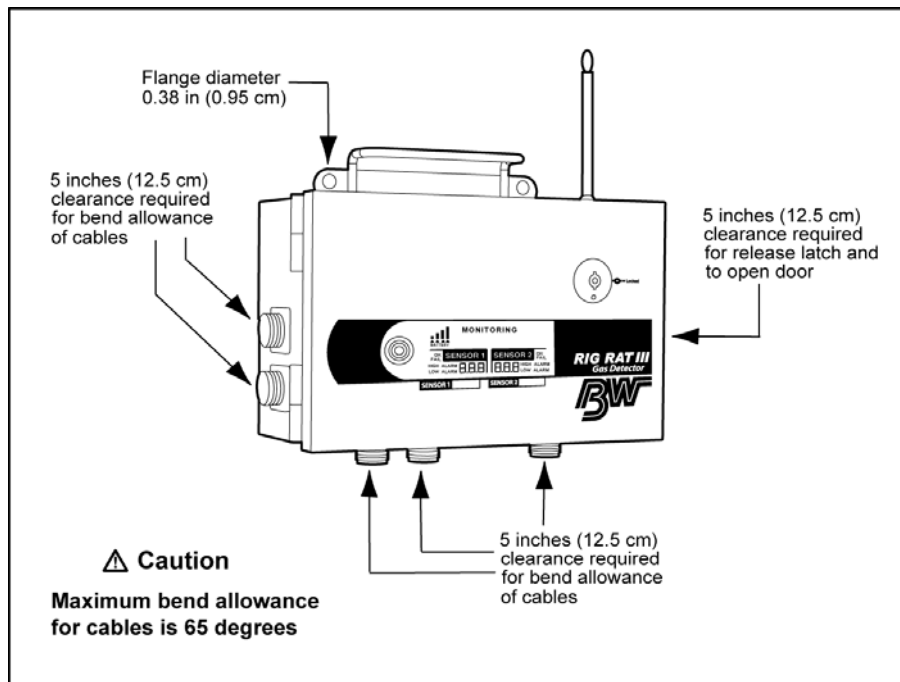


Figure 6. Mounting Requirements

Installation

⚠ Caution

Only qualified personnel should perform installations. Install detectors according to applicable electrical codes, regulations, and safety standards. Ensure that correct cabling and seal fitting practices are implemented.

Installation Location

Radio signals transmit well over flat terrain and open water. However, buildings, metal tanks, and other obstructions can interrupt radio transmissions.

When determining a location for the detector, consider

- the terrain,
- obstructions (such as buildings and metal tanks),
- line-of-sight to the controller antenna (if used with a controller),
- radio frequency interference (RFI), and
- if the detector is used for confined space detection.

Read the following sections, [The Detector](#) and [The Antenna](#) prior to determining the location for installing the detector.

The Detector

Before installing the detector,

- ensure that it is located in an area where it is not exposed to electrical or severe mechanical shock, and
- determine if it will be used to monitor a confined space.

Confined Space: For continuous confined space monitoring and pre-entry protection, install the detector approximately 5 to 6 ft. above ground outside the entrance of the building.




Figure 7. Confined Space Installation

Installing the detector at a lower level requires a high gain antenna. Refer to [The Antenna](#) for more information.

Drill 1.5 inch (3.8 cm) access holes below the detector for the sensor cables and for the remote option cable.

The Antenna

As well as determining the optimum location for the detector, the antenna also has specific requirements. BW recommends that the antenna

- not be located near water,
- is positioned well above surrounding objects,
- maintains a clear line-of-sight to the controller (if used with a controller), and
- be placed as far as possible from other antenna systems to avoid possible Radio Frequency Interference (RFI).

For transmission distances, refer to [Specifications](#) and any applicable accessory manuals.

Low Gain Antenna: The low gain antenna is used for shorter distances without obstructions and with a clear line of sight to the controller.

High Gain Antenna: The high gain antenna is used for greater transmission distances and is used to extend above obstructions.

Note

Atmospheric conditions may cause signal loss.

⚠ Warning

Use extreme caution when working near telephone and electrical power lines. Always mount the antenna two times its length (minimum) away from power lines.

The detector is equipped with a TNC antenna port. Install the antenna and all required extension cables.

Antenna Cable: Antenna cable lengths must be less than 20 ft. (6 m). LMR 240 cable is provided with the detector. For greater transmission distances, use heavier cable such as, the LMR 400.

Refer to Antenna/Cable Assembly/Mounting Brackets in [Replacement Parts and Accessories](#).

Note

The use of mating connectors to extend cable lengths is not recommended.

Connectors cause signal strength loss and shorten transmission distance.

Mounting the Detector

Note

Install the detector vertically with the antenna pointing upwards only.

The detector is equipped with pre-drilled mounting flanges for permanent installation. The required minimum/maximum clearances are as follows:

- Maintain a minimum clearance of 0.38 in. (0.95 cm) below and from each side of the detector.
- Maintain a maximum 65° bend allowance for all cables connected to the detector.

Refer to Figure 6. Mounting Requirements. Installation bolts are included in the Rig Rat III Detector kit.

Cable Installation

Separate cables are required for each detector. All connections must be installed using shielded cable only.

Warning

In classified areas, use only hazardous location cable. Use shielded cable only.

Table 10. System Cable Connection

Cable Type	Identifier	# of Pins	Female Connector Mates with	Male Connector Mates with
Sensor	orange ends	6	detector sensor port	sensor head
Solar panel	yellow jacket	5	charger	detector charger port
Option	various	6	option device	detector option port

Note

For installation of an unapproved charger or option device in a Class I, Div. 1 area, refer to [Appendix B Installation Requirements](#).

Grounding the Detector

Warning

The detector must be grounded. Correct grounding practices reduce equipment damage and improve safe working conditions.

It is extremely important that the detector be grounded to ensure Intrinsic Safety and optimum system operation. After determining where to mount the detector, it must be grounded accordingly.

To determine the grounding requirements, refer to the following four installation grounding conditions and procedures.

- [Condition 1: Mount is Metallic and at Earth Ground Potential](#)
- [Condition 2: Mount is Non-Metallic \(Non-conducting\)](#)
- [Condition 3: Mount is Metallic but Not Grounded to Earth Ground \(Non-conducting\)](#)
- [Condition 4: Plant Ground Rod is Not Available and an Earth Ground Must Be Provided](#)

Note

All system components and plug-in option devices are bonded to the main system through the connecting cables.

To prevent Radio Frequency Interference (RFI), ensure that all permanent equipment that uses radio signal communication is grounded, such as base stations.

Installation Grounding Conditions

Condition 1: Mount is Metallic and At Earth Ground Potential

1. Examine the bond between the mount and the earth ground.

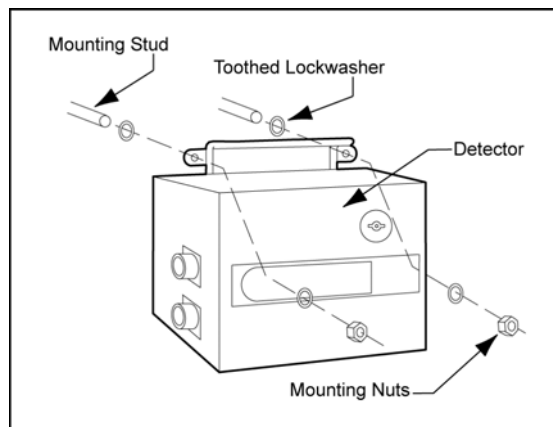


Figure 8. Bonding the Detector

2. Use toothed lock washers to achieve a system bond. Refer to Figure 8. Bonding the Detector.

Condition 2: Mount Is Non-metallic (Non-conducting)

1. Determine a plant ground location.
2. Using a bonding cable (4-12 gauge insulated wire), connect to the existing plant ground network.

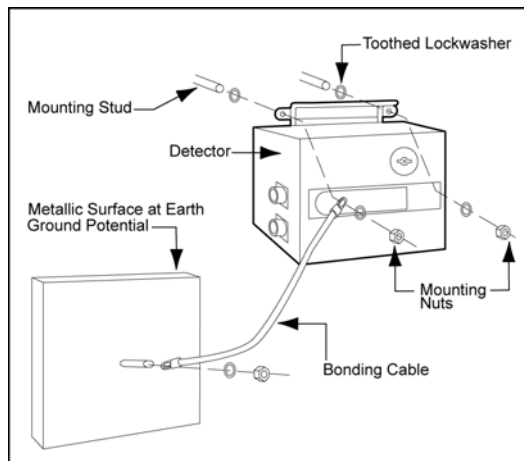


Figure 9. Bonding with Bonding Cable

3. Mount the system components in location, and connect the other end of the bonding cable to the mounting bracket. Refer to Figure 9. Bond with Bonding Cable.

Condition 3: Mount is Metallic, but not Grounded to Earth Ground (Non-conducting)

1. If the location is not correctly grounded, a ground must be supplied.
2. Using toothed lock washers, mount the detector in the selected location.
3. If a plant ground is not available, complete the procedures in [Condition 2](#) or establish an earth ground as in [Condition 4](#).

Condition 4: A Plant Ground Rod is Not Available and Earth Ground Must Be Provided

1. Drive a grounding rod into the earth approximately 2 ft. (0.66 m).
2. Secure a bonding cable (4-12 gauge insulated wire) between the detector and the grounding rod as shown in Figure 10. Grounding Rod Installation.

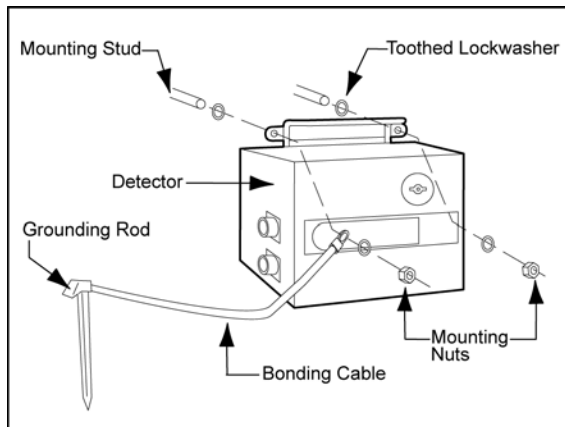


Figure 10. Grounding Rod Installation

Setting the Detector and Transceiver Channels

Digitally coded information is received via 2.4 GHz radio using Frequency Hopping Spread Spectrum Technology.

The detector and transceiver channels can be set while the detector is activated or deactivated. The channels can be changed on site when

- moving detectors,
- adding detection points, and/or
- replacing equipment.

To set the detector and transceiver channels to enable communication between the detector and the controller, complete the following:

1. Unlatch, unlock, and open the exterior door.
2. If the detector is activated, complete steps #3-5.
If the detector is deactivated, complete steps #4-5.
3. On the operations bay door, press ☐ XMTR DISABLE. Refer to Figure 2.

4. Remove the two Phillips screws from the operations bay door.
5. Locate the RIG RAT III Transceiver. Refer to Figure 11.

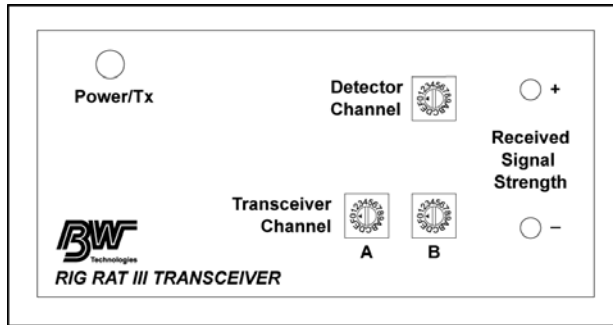


Figure 11. RIG RAT III Transceiver

Detector Channel: Only channels 1-4 are available to select from. If channels 5-9 or A-F are selected, they will be recognized as channel 1.

The detector's transceiver operates in transmit mode if the channel rotary switch is positioned to any channel except channel 0.

Use a small flathead screwdriver to turn the rotary switch. Position the arrow towards the required channel.



Figure 12. Channel Rotary Switch

Transceiver Channels: To set the transceiver channels, complete the following:

6. Using the rotary switches located above A and B, position the arrows to the required channels. The available channels are 00 to 3F.

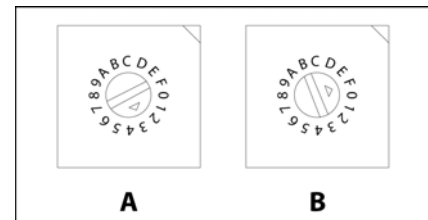




Figure 13. Transceiver A and B Channels

Important: The transceiver channel(s) on the detector(s) must be set to the same transceiver channel on the controller. There is a maximum of four detectors per controller.

7. Set the transceiver channel on the detector.
8. Set the transceiver channel on the controller. Ensure that it is set to the same channel as the detector.

Refer to the Rig Rat III Controller User Manual for procedures.

9. On the detector, press  XMTR DISABLE.
10. On the detector, press  XMTR TEST. Both the detector and controller LCDs display the count down from **999 999** to **000 000**.
11. Deactivate and then reactivate the detector to confirm the channel selection, otherwise the detector will not recognize the selection/change.

The Sensors

Sensor Locations

There are several factors to consider when selecting a location to install the sensor(s). Refer to the following recommendations to ensure accurate gas detection.

Air Currents: If there are fans, wind, or other sources of air movement, gases may rise or collect in some areas.

Gas Density: To detect gases that are lighter than air, install the sensor approximately 12 in. (30 cm) above the potential gas release. For indoor installations, install the sensor near the ceiling.

To detect gases that are heavier than air, install the sensor approximately 12 in. (30 cm) below the release level. If there are no air currents in the area, install the sensor near the floor or ground.

Gases with a density equal to or slightly greater than air typically rise, especially when there are air currents.

Gas Emission Sources: A minimum of one sensor must be located near each point where a leak is likely to occur, especially when a low volatile liquid is being monitored.

Environmental Factors: Although the sensors are designed for outdoor use, install sensors where they will be protected from

- wind,
- dust,
- snow,
- water,
- vibration, and/or
- electrical/mechanical shock.

Adhere to the temperature operating range of the sensor. Refer to [Encapsulated Sensor Specifications](#) in [Appendix A](#) and/or [Stainless Steel Sensor Specifications](#) in [Appendix C](#).

Sensor Installation

The sensor is linked to the detector using RFI/EMI shielded cable that connects directly to both the sensor (male) and the detector (female). Each cable is constructed with a label that lists the cable length.

Cable lengths

- Toxic sensor up to 250 ft. (76.2 m)
- Combustible sensor up to 100 ft. (30.5 m)

When installing the sensors, ensure that

- the cable connectors are clean and not damaged for proper connection,
- each sensor and connecting cable is connected to the correct port (SENSOR PORT 1 or SENSOR PORT 2) that is located on the left side of the detector.

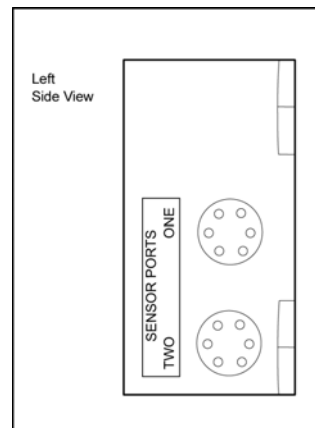


Figure 14. Sensor Ports on Detector

Note

Cable bend allowances must not exceed 65°.

To install the sensor(s), complete the following:

1. Connect the sensor cable(s) to the desired sensor port(s).

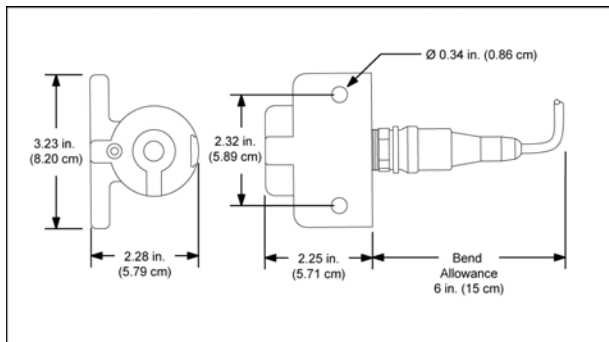


Figure 15. Sensor Dimensions (Encapsulated)

2. Secure the sensor at the desired location. It can be bolted, screwed, or clamped in place. The optional tripod has predrilled mounts on the legs to attach the sensors.
3. Ensure that the sensor head is directed to the side or downwards to prevent dirt, debris, water, or snow from accumulating on the sensor screen.

4. Connect the sensor cable to the sensor. Hand tighten the crown connector on the cable to the sensor to ensure a weatherproof seal and proper connection.
5. On the external door of the detector, paste labels beside or below the SENSOR 1 and SENSOR 2 markers. Record the gas type and the measuring range. Refer to Figure 16.

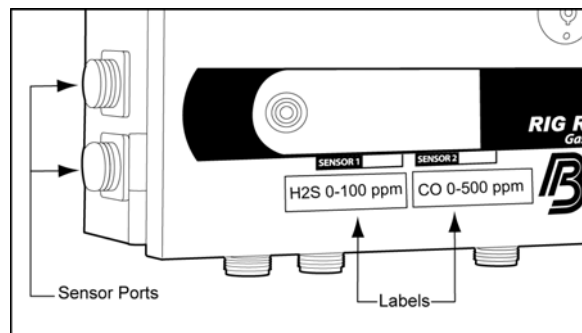


Figure 16. Labeling the Sensors on the Detector

Note

A factory gas type label is attached to each sensor.

Sensor Measuring Ranges

The gas type measuring range(s) are set on the main board of the detector (Figure 3).

To set a sensor measuring range, complete the following:

1. Open the exterior door and open the operations bay door. The main board is located on the inside of the operations bay panel.

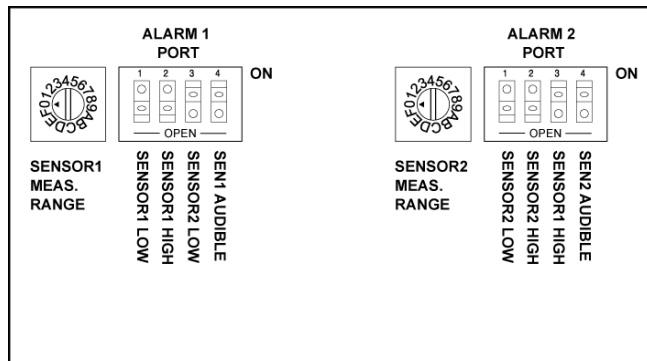


Figure 17. Sensor Measuring Range Rotary Switches

2. On the main board, locate the SENSOR 1 MEAS. RANGE and SENSOR 2 MEAS. RANGE rotary switches (Figure 17).

Each number and letter on the rotary switch is configured to display the measurement (example: **0-100 ppm**) on the detector LCD.

3. Refer to [Encapsulated Sensor Measuring Ranges](#) and/or [Stainless Steel Sensor Measuring Ranges](#) to determine the correct measuring range(s) for the corresponding sensor(s).
4. Using a small flathead screwdriver, position the rotary switches to set the sensor measuring ranges. View the detector LCD while turning the rotary switch until the correct measuring range displays.

Or

Refer to Table 11. Sensor Measuring Range Selection and the following examples.

Note

*Rotary switch position 0 (zero) is used to disable the sensor. Position 0 displays as **OFF** on the detector LCD.*

Table 11. Sensor Measuring Range Selection

Switch Position	LCD Measuring Range	LCD Resolution
0	Sensor Disabled	OFF
1	0 – 100	1
2	0 – 10	1
3	0 – 1.00	0.01
4	0 – 9.99	0.01
5	0 – 200	1
6	0 – 20	1
7	0 – 2.00	0.01
8	0 – 20.0	0.1
9	0 – 500	1
A	0 – 50	1
B	0 – 5.00	0.01
C	0 – 50.0	0.1
D	0 – 999	1
E	0 – 30.0 (En./Def.)	0.1
F	0 – 30.0 (Def./Def.)	0.1

Example 1: For 0-100 ppm H₂S or 0-100% LEL, set the switch to position 1 (**0-100**).

Example 2: For 0-500 ppm CO, set the switch to position 9 (**0-500**).

If the measuring range of the sensor is not listed in Table 11, select the next highest measuring range.

Important:

Switch E: low alarm = enrichment, high alarm = deficiency
Switch F: low and high alarm = deficiency

Installing Optional Devices/Accessories

Refer to all corresponding installation manual(s) for any additional devices/accessories that are installed.

Warning

To install an Intrinsically Safe system, adhere to all safety regulations. For installation of unapproved accessories in a Class I, Div. 1, Group C, D area, refer to [Appendix B Installation Requirements](#).

Independent Power

The detector and rechargeable option devices use the same low maintenance batteries.

The power options that are provided enable the detector to

- operate from the internal battery, or
- trickle charge the system for maintenance-free operation.

Trickle Charge Options

- Solar power 5, 10, 20, or 30 watt panels
- 24 Vdc direct line power
- 110 or 220 Vac line power
(using a BW 24V output trickle charger)

A detector that is powered by the internal 12 V, 3 amp hour battery and equipped with the sensor types listed in Table 12, provides the following days of operation:

Table 12. Sensor Types and Battery Life

Number of Sensors	Type of Sensor	Days of Operation
2	Toxic or O ₂	21
1	Toxic or O ₂ plus combustible	3.5
2	LEL (combustible)	2.0
1	Toxic or O ₂	28.0

Battery Life

Battery life is also dependant upon the following:

- The transmission interval that is set during calibration (frequent transmissions reduce the battery life).
- The power draw of rechargeable option devices and field interfaces can reduce battery life.
- A 10 watt solar panel (minimum) is required to trickle charge a detector that is equipped with one or two combustible sensors.
- In a line or solar powered situation, the battery provides the backup in the event of a power interruption.

For additional charger installation information, refer to [Appendix B Installation Requirements](#).

Battery Level

Ensure that the battery has obtained a full charge. The battery level displays continuously on the detector LCD.

Low Battery Level: If the battery level is low, the battery level indicator displays below the lowest bar.

Very Low Battery Level: If the battery level is too low (below 10 V), only the battery levels icon displays on the LCD (no other data displays).

Depleted Battery Level: If the battery level drops below 9.5 V, the detector automatically deactivates.

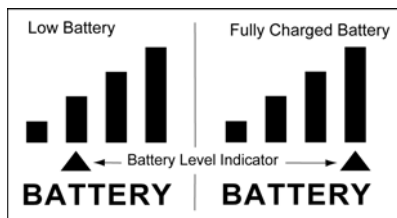


Figure 18. Battery Levels

In either situation, use the BW bench charger to charge the detector battery immediately.

Line Power

⚠ Caution

Only qualified personnel should perform power installations. Installations must be performed according to applicable electrical codes, regulations, and safety standards.

Installation: 24 Vdc direct and ac line power.


The detector and all BW rechargeable option devices can be trickle charged directly using line power (24 Vdc, 115 and 230 Vac). The detector fuse protects against power fluctuations.

Charger Power

Install a charger (if applicable): Solar panels or 110/220 Vac or 24 Vdc direct line chargers. Refer to [Appendix B Installation Requirements](#).

Applying Power

Press the XMTR DISABLE button to prevent false alarms at the controller during detector power up and setup.

Once all the equipment is installed and source of power is selected, press  POWER to apply power to the detector.

Sensor Readout Status

If an alarm condition occurs while activating the detector, verify that the

- correct sensor measuring range (rotary switch setting) has been selected, and
- sensors are correctly installed.

Note

*Even if the transmitter is disabled, during an alarm condition the red LED alarm on the operations bay panel flashes and **DANGER** displays on the LCD.*

Allow the sensors adequate time to stabilize prior to monitoring gases. Refer to Table 13. Sensor Stabilization for required times.

Table 13. Sensor Stabilization

Sensor	Condition	Time to Stabilize
Common (most sensors)	Normal	2 minutes
Common (most sensors)	Extreme temperatures	2 minutes plus (times will vary)
Biased <ul style="list-style-type: none">• Ethanol• Ethylene oxide• Hydrogen chloride• Nitric oxide	All conditions	24 hours

Calibration and Setting Alarm Setpoints

Guidelines

When calibrating the sensors, adhere to the following guidelines.

- Refer to [Appendix A: Encapsulated Sensors](#) and/or [Appendix C: Stainless Steel Sensors](#) for recommended gas mixtures and flow rates.
- Calibration accuracy is never better than calibration gas accuracy. Use a premium-grade calibration gas. Gases with National Institute of Standards and Technology (NIST) traceable accuracy improves the validity of the calibration.
- Calibrate toxic and O₂ sensors with gas. Refer to [Appendix A: Encapsulated Sensors](#) and/or [Appendix C: Stainless Steel Sensors](#).
- Do not use a gas cylinder beyond its expiration date.
- Calibrate the sensors at least once every 90 days (3 months), depending upon the use and exposure to poisons and contaminants.

- Calibrate the sensors if they are returned to use after being in storage.
- Calibrate a new sensor before use. Allow the sensor to stabilize before starting calibration. Refer to Table 13 Sensor Stallization.

When to Calibrate

Calibrations are performed to adjust the sensitivity levels of the sensor to ensure accurate responses to gas.

It is necessary to calibrate the sensor(s) and set the alarm setpoints after

- completing the initial installation,
- installing a new sensor,
- returning the system and sensors to use after being in storage, and
- regular use (calibrate every 90 days).

Calibration Features

When activating, allow the detector and sensors a minimum of 2 minutes to stabilize before performing calibration.

Note

Some sensor types require a longer period of time to stabilize such as ethanol, ethylene oxide, and nitric oxide. For more information, refer to [Appendix A Encapsulated Sensors](#) and/or [Appendix C Stainless Steel Sensors](#).

From the calibration function, modifications can be made to the

- low and high alarm setpoints,
- calibration gas concentration levels,
- transmission intervals, and
- loss of transmission intervals.

Table 14. Default Factory Settings

Description	Factory Setting
Sensor1 low alarm	25
Sensor1 high alarm	50
Sensor1 zero adjust	00
Sensor1 span adjust	50
Sensor2 low alarm	25
Sensor2 high alarm	50
Sensor2 zero adjust	00
Sensor2 span adjust	50
Hour time interval	00h
Minute time interval	00.
Second Time interval	.05
Hour time expired	00h
Minute time expired	1.

Setting the Alarm Setpoints

Calibrations are performed to adjust the sensitivity levels of the sensors to ensure accurate responses to gas.

To calibrate the sensor(s) and set the alarm setpoints, complete the following:


Note

If only one setpoint is required, set both the low and high alarm setpoints to the same value.

1. Refer to [Encapsulated Sensor Measuring Ranges](#) and/or [Stainless Steel Sensor Measuring Ranges](#) to determine the correct ranges.

The alarm setpoints can be set to any value within the designated range limit for the sensor.

2. On the detector operations bay panel, press ☐ LOW/▼ to display the current low alarm setpoint(s).

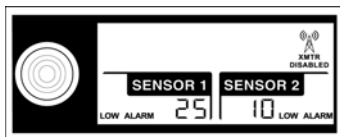

3. Press ☐ HIGH/▲ to display the current high alarm setpoint(s).



To change the low and/or high alarm setpoints, complete the following:

4. Enter calibration mode by pressing ☐ LOW/▼ and ☐ OK simultaneously.

The value for the **SENSOR 1 LOW ALARM** displays.

5. To change this setpoint(s) press ☐ LOW/▼ or ☐ HIGH/▲ until the desired value displays.

Or

To retain the current setpoint(s) value, press ☐ OK.

6. If a new value is selected, press ☐ OK to confirm the change. Set the high alarm setpoint if required.

7. If required, repeat steps #1-6 for the remaining sensor.

Note

Oxygen can be set to have both a deficient and an enrichment alarm.

Calibrating Stainless Steel Sensors

Refer to [Calibration \(Stainless Steel Sensors\)](#) step #8 in [Appendix C](#).

Calibrating Encapsulated Sensors

The encapsulated sensor is factory calibrated (zeroed) and ready for installation; however, after several uses drift can occur. The sensor must then be calibrated.

If the sensor requires calibration, complete [Auto Calibration](#) steps #8-9 before proceeding to [Auto Span](#).

⚠ Caution

Perform the following calibration procedures in a clean atmosphere that is free of hazardous gas.

Auto Calibration

8. Using the pen magnet, place it in the magnet area as shown in Figure 21.

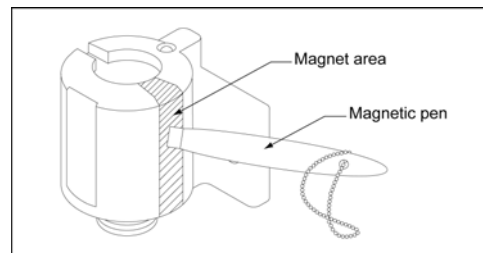


Figure 21. Sensor Magnet and Magnetic Pen

The sensor LED blinks to indicate that the magnetic pen is being held in the correct location on the sensor. Continue to hold the pen in place.

The sensor continues to blink for approximately 5 seconds.

9. When the sensor has been successfully auto calibrated, the LED stops blinking. Remove the magnetic pen.


Successful Auto Calibration: If the detector displays a 0% LEL reading, proceed to step [Auto Span](#) step #10.

Unsuccessful Auto Calibration: If the detector does not display a 0% LEL reading, the detector must then be auto zeroed. Complete the following:

Rig Rat III Detector

User Manual

From the operations bay panel, press ☐ LOW/▼ or ☐ HIGH/▲ until 0 (zero) displays on the detector LCD.

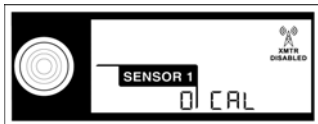

Press ☐ OK to accept the new value.

Note

Zero drift for the O₂ sensor is extremely minimal over the life span of the sensor. If zeroing is required, apply 100% Nitrogen (N₂).

When the detector is successfully auto zeroed, return to [Auto Calibration](#) step #8 and auto calibrate the sensor again before proceeding to [Span the Sensor and Detector](#), step #14.

Auto Span

Refer to [Encapsulated Sensor Measuring Ranges](#) for recommended gas mixtures and flow rates before continuing.

Auto span requires approximately 90 seconds to complete.

10. Place the calibration cap onto the sensor head.

To ensure uniform gas flow, the inlet/outlet of the cap must be horizontally aligned with the main outlet of the sensor head exactly as shown in Figure 19.

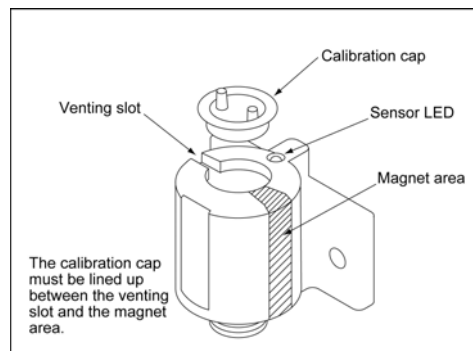


Figure 19. Calibrating the Encapsulated Sensor

11. When the sensor is ready for calibration gas, the sensor LED blinks once every second.
12. Connect the tubing to the cylinder and to the calibration cap as shown in Figure 20.

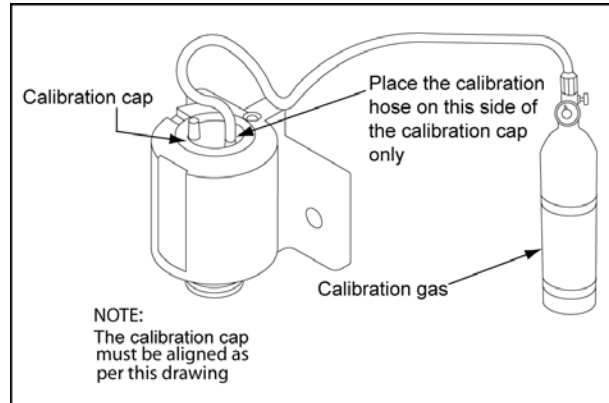


Figure 20. Calibration Connections

13. Apply the gas to the sensor. When the auto span is complete the sensor stops blinking.

Successful Auto Span: The detector displays approximately 50% LEL. Proceed to [Span the Sensor and Detector](#), step #14.

Unsuccessful Auto Span: If the detector does not display approximately 50% LEL, auto zero the detector and auto calibrate the sensor again.


Note

If the sensor response from the calibration gas is less than 15% LEL, the calibration has failed. The sensor LED blinks fast for 2 seconds to indicate the fail.

Span the Sensor and Detector

14. Insert the calibration cap and open the valve on the cylinder. Apply a known concentration of gas to the sensor until the detector LCD readout stabilizes (approximately 2 minutes).

The detector must display the same concentration value as the calibration gas being used.

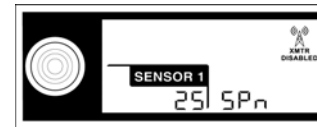

15. To adjust the concentration value on the detector, press ☐ LOW/▼ or ☐ HIGH/▲ until the required value displays.
16. Press ☐ OK to accept the new value.

17. Remove the gas from the sensor and close the valve of the gas cylinder. Allow the detector time to display a zero reading.

Detector Does Not Return to Zero Reading: If the sensor reading does not return to zero, ensure the sensor measuring range rotary switch is set correctly.

Reset the rotary switch if required and repeat the calibration procedures. Repeat the calibration procedures for SENSOR 2 (if applicable) before setting the [Transmission Interval](#).

Calibration Successful: Proceed to [Transmission Interval](#).

Calibration Unsuccessful: After calibration, if the sensor LED blinks every 2 seconds, the calibration has failed. Re-calibrate the sensor. If calibration fails again, contact [BW Technologies](#).

Transmission Interval

Note

Before proceeding, ensure that both SENSOR 1 and SENSOR 2 (if applicable) have been calibrated.

The transmission interval is used to set the detector to transmit data to the controller on a regularly scheduled basis. The detector can be set to transmit data once a day, hourly, or more frequently.

- Minimum 5 seconds
- Maximum 25 hours

To set/change the transmission time, complete the following:


18. Determine how frequently the transmissions are to be sent to the controller.

Note

Frequent transmissions require that the battery be recharged more frequently.

19. From the detector, press ☐ LOW/▼ and ☐ OK simultaneously to enter calibration mode (if required).
20. From calibration mode, press ☐ LOW/▼ and ☐ OK simultaneously again to access the transmission time screen.


The hours **00h** interval screen initially displays.

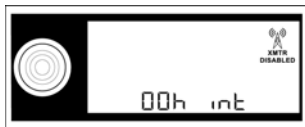

21. Press ☐ LOW/▼ or ☐ HIGH/▲ until the required hour(s) value displays (maximum 25 hours).
22. Press ☐ OK to accept the new value.

Or

For more frequent transmissions (less than 1 hour), press ☐ OK to bypass and automatically access the minutes **00.** interval screen.

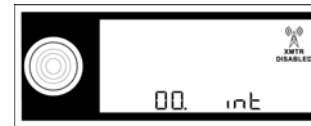

23. Press ☐ LOW/▼ or ☐ HIGH/▲ until the required minute(s) value displays.
24. Press ☐ OK to accept the new value.

Or

For more frequent transmissions (less than 1 minute), press ☐ OK to bypass and automatically access the seconds **.00** interval screen.




25. Press ☐ LOW/▼ or ☐ HIGH/▲ until the required seconds value displays (minimum .05 seconds).

26. Press ☐ OK to accept the new value.

The loss of transmission time interval screen
00h t.E displays.

Loss of Transmission Time Interval

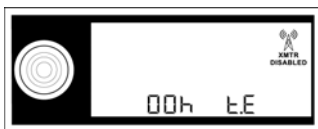

In the event that transmissions are interrupted, this function is used to enter a specified time that a controller will wait for transmissions from a detector before entering an alarm state.


- Maximum period of standby: 97 hours
- Minimum period of standby: 1 minute

To enter a loss of transmission time interval, complete the following:

27. The initial loss of transmission time interval (**00h t.E**) screen displays the hours (**00h**). Press ☐ LOW/▼ or ☐ HIGH/▲ until the desired hour(s) value displays.
28. Press ☐ OK to accept the new value.

Or

For reduced transmission time interval (less than 1 hour), press ☐ OK to bypass and automatically access the minutes (**00. t.E**) screen.

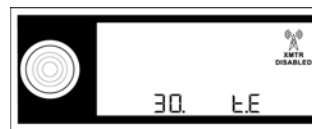

29. Press ☐ LOW/▼ or ☐ HIGH/▲ until the desired minute(s) value displays.
30. Press ☐ OK to accept the new value.

The end calibration screen displays.

End Calibration



After the loss of transmission time interval is set, the LCD displays **End CAL** to signal the end of the calibration procedure.

Alarms

The following table describes the system alarms and shows how the LCD displays for each alarm. Alarms automatically reset to normal operation when an alarm condition no longer exists.

Table 15. Alarms


Alarms	Display
<p>Low Gas Alarm</p> <ul style="list-style-type: none"> Transceiver transmits every 10 seconds Red LED flashes DANGER displays and flashes LOW ALARM displays to indicate the alarm level and displays below the sensor that is affected LCD displays the numeric value of the detected gas Audible alarm sounds (if enabled) Option devices attached to the OPTION PORTS activate (if enabled) 	

Table 15. Alarms


Alarms	Display
<p>High Gas Alarm</p> <ul style="list-style-type: none">• Transceiver transmits every 10 seconds• Red LED flashes• DANGER displays and flashes• HIGH ALARM displays to indicate the alarm level and displays below the sensor that is affected• LCD displays the numeric value of the detected gas• Audible alarm sounds (if enabled)• Option devices attached to the OPTION PORTS activate (if enabled)	

Table 15. Alarms

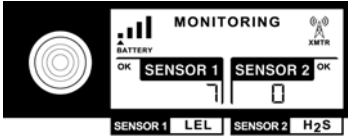
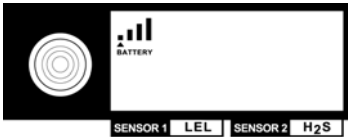
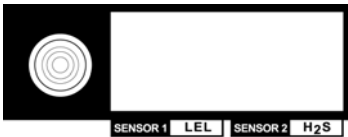

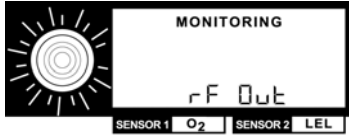
Alarm	Display
<p>Low Battery Alarm (1)</p> <ul style="list-style-type: none"> Transceiver transmits every 10 seconds Battery level indicator displays below the lowest bar 	
<p>Very Low Battery Alarm (2)</p> <ul style="list-style-type: none"> If the battery level drops below 10 V, only the flashing battery level displays. 	
<p>Depleted Battery Alarm (3)</p> <ul style="list-style-type: none"> If the battery level drops below 9.5 V, the detector automatically deactivates. 	

Table 15. Alarms


Alarm	Display
Sensor Integrity Alarm <ul style="list-style-type: none"> • XMTR alarms activate • Red LED flashes • DANGER displays and flashes • FAIL displays beside the sensor that is affected • Audible alarm sounds • Option device(s) configured for the sensor(s) activates 	 <p>The display shows a sun icon on the left. The main area contains the word 'MONITORING' at the top, followed by 'DANGER' in large letters. Below 'DANGER' are two sensor status boxes: 'SENSOR 1' with a 'FAIL' indicator and 'SENSOR 2' with an 'OK' indicator. At the bottom, there are two small boxes labeled 'SENSOR 1' and 'SENSOR 2' with 'O2' and 'LEL' respectively.</p>
Loss of Transmission Alarm <ul style="list-style-type: none"> • Red LED flashes • LCD displays rF Out • Audible alarm sounds after several transmission fails • Option devices attached to the OPTION PORTS activate (if enabled) 	 <p>The display shows a sun icon on the left. The main area contains the word 'MONITORING' at the top, followed by 'rF Out' in large letters. At the bottom, there are two small boxes labeled 'SENSOR 1' and 'SENSOR 2' with 'O2' and 'LEL' respectively.</p>

Viewing the Maximum Gas Level


The maximum gas level feature indicates the maximum gas exposure encountered.

To view the maximum gas level, complete the following:

1. Press and hold ☐ HIGH/▲ and ☐ OK simultaneously for 1 second.

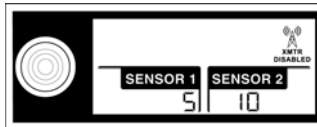

2. To clear the maximum gas level detected, press and hold ☐ HIGH/▲ and ☐ OK simultaneously for 5 seconds until **CLr** displays on the LCD.

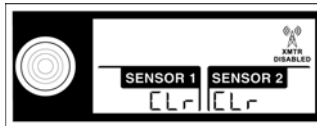

Setting Dipswitches for Alarm Options

The detector can be set to engage different alarm options devices (sirens, strobe lights, audible alarms, etc.) when the

low and high alarm setpoints are exceeded by setting the option port dipswitches.

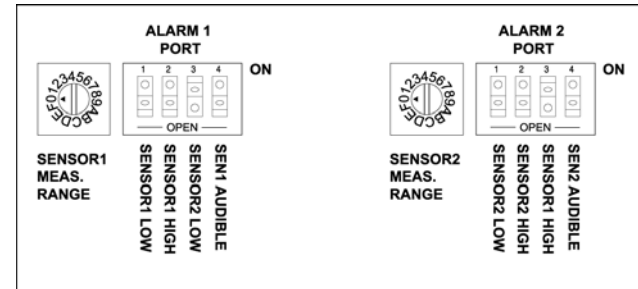


Figure 22. Measuring Range Dip Switches

The option port dipswitches are used to enable/disable the OPTION PORTS (ONE and TWO) that are located on the bottom of the detector. Option devices that can be connected are

- audible alarm devices,
- visual alarm devices,
- relay devices, and
- solenoid drivers.

The ALARM 1 PORT and ALARM 2 PORT dip switches are positioned on the main board (Figure 22) that is located inside the internal components bay of the detector (Figure 3).

To access the main board, remove the two screws from the operations bay panel to open. The main board is attached to the inside of the operations bay panel.

Table 16. Default Alarm Dip Switch Settings

Description	Factory Setting
0 = off	1 = on
Sensor 1 Audible	1
Sensor 2 Low	0
Sensor 1 High	1
Sensor 1 Low	1
Sensor 2 Audible	1
Sensor 1 High	0
Sensor 2 High	1
Sensor 2 Low	1

To set the alarm port dip switches, refer to Table 17. Alarm Dip Switch Settings and the following Examples 1-3.

Example 1: One sensor using two alarm ports
ALARM 1 PORT engages when SENSOR 1 is in low alarm.
ALARM 2 PORT engages when SENSOR 1 is in high alarm.

Table 17. Alarm Dip Switch Settings

Alarm 1 Port					Alarm 2 Port			
S1 = sensor one S2 = sensor two Ex = Example 0 = off 1 = on					L = low alarm H = high alarm A = audible alarm			
	S1L	S1H	S2L	S1A	S2L	S2H	S1H	S2A
Ex 1	1	0	0	1	0	0	1	0
Ex 2	1	1	0	1	1	1	0	1
Ex 3	1	0	1	1	0	1	1	1

Example 2: Two sensors using one alarm port
ALARM 1 PORT engages when SENSOR 1 is in low or high alarm.
ALARM 2 PORT engages when SENSOR 2 is in low or high alarm.

Example 3: Two sensors using two alarm ports
ALARM 1 PORT engages when SENSOR 1 and SENSOR 2 are in low alarm.
ALARM 2 PORT engages when SENSOR 1 and SENSOR 2 are in high alarm.

The dipswitches activate the connected option devices via the pins in the connector ports. They are as follows:

- ALARM1 PORT dipswitch activates pin A of OPTION PORT ONE and OPTION PORT TWO.
- ALARM2 PORT dipswitch activates pin B of OPTION PORT ONE and OPTION PORT TWO.

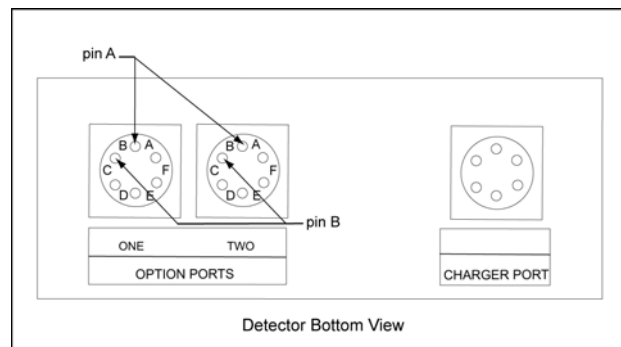


Figure 23. Pin A and Pin B Option Ports

Alarm Option Features and Exceptions

Features

- The audible alarm for sensor 1 (S1A) and sensor 2 (S2A) can be enabled for both low and high alarms.

- The sensor integrity alarm engages all alarms and all connected option devices.
- The alarms automatically reset when alarm conditions no longer exist.

Exceptions

The UR-L601 and UR-L602 strobe option devices are

- alarm level specific in a single sensor application, and
- sensor specific in a dual sensor application.

Maintenance

System Components: All electronics are sealed in weatherproof enclosures. However, regular maintenance is required for all system components. Visually inspect and test regularly to ensure optimum performance.

Sensors: The sensors are exposed to the environment and must be calibrated minimum every 90 days (3 months) to ensure accurate detection of gas.

Ensure the sensor screen is clean and not damaged. Clean the screen(s) if required. Do not paint the sensor enclosures.

Do not use any type of solvent to clean the sensors.

Maintenance Log: Maintain an accurate maintenance log of

- calibration dates,
- sensor replacements, and
- other service/events/occurrences.

Detector: Ensure that the exterior door and the operations bay panel are closed correctly and secured. Ensure that cover caps are securely fastened to all ports not in use. Check the battery level at regular intervals.

To ensure a weatherproof seal, confirm that the exterior door clasp is securely fastened.

Antennas: Replace any bent or damaged antenna extension cables. Periodically test the transmission.

Controllers: Refer to the controller user manual.

Remote Plug-in Cables: Inspect all of the cables regularly. Ensure that all cables are connected correctly. Replace cables that are damaged.

Replacing the Fuse (500mA)

If the 500mA fuse on the main board requires replacement, contact [BW Technologies](#).

Storage and Transport

BW batteries have a low rate of self discharge. Therefore, the battery powered instruments can be used irregularly or can be stored for long periods of time.

When storing or transporting battery powered equipment, be aware that

- the equipment must be stored in a warm area as freezing the electrolyte damages the battery (as the battery discharges, the battery freezing point rises),
- the rate of discharge varies with storage temperature,
- higher temperatures result in a faster discharge rate, which reduces the time that the equipment can be stored, and
- the battery level should not drain below 50% of the fully charged state.

Prior to Storage or Transport

Caution

Completely discharged batteries must be charged within 30 days.

Adhere to the following:

- If the battery is completely discharged for a long period of time, cycle charge the unit several times to restore function.
- Ensure that the equipment is fully charged before returning to service. Depending upon the conditions, cycle charging may restore up to 75% of full charge.
- Ensure that all instruments are fully charged before storing or transporting.

To prepare equipment for storage or transport, complete the following:

1. Deactivate the required equipment.
2. Create a record of the current connections. This ensures that the equipment is reassembled correctly.

Record the removal date of the sensors, option devices, accessories, and the detector.

3. Disconnect the following from the detector:

- Sensor(s)
- Option devices
- Charger
- Cables

4. Replace all cover caps for the ports located on the side and bottom of the detector.

5. Loosely coil and secure all cables to prevent damage.

6. Insert a calibration cap on each sensor.

Important: Detectors and rechargeable option devices should be recharged at least once every 6 months when in storage.

System Test

After installing the detector, option devices, and setting the dip and rotary switches, it is essential to complete all of the following tests to ensure that the system responds correctly in the event of an alarm condition.

System tests should also be performed when


- the system or a detector is moved,
- sensors are changed/added,
- sensor measuring range(s) are changed, and
- option devices are added/changed.

Important: Test each detector on the system (system = one to four detectors per controller).

To perform a system test, complete the following:

1. Activate the detector(s) and the controller.

Test Signal Transmission and Reception

2. On the detector, press  XMTR TEST to verify the transmission and reception signals.



Both the detector and the controller LCDs display a count down from **999 999** to **000 000**.



Test Sensor Integrity Alarm

If the signal from the sensor is disrupted (sensor or sensor cable is disconnected or damaged), the detector engages the sensor integrity alarm.

To test the integrity alarm, complete the following:

3. Disconnect the sensor from the detector.
4. Ensure the following actions occur:
 - the transmitter alarm engages and sends a signal to the controller,
 - the controller receives the signal,
 - the red LED lights and flashes on the detector,
 - **DANGER** displays and flashes on the detector LCD,
 - **FAIL** displays on the detector LCD below the sensor that has been disconnected,
 - the audible alarm sounds, and
 - all additional alarm option devices engage.
5. After confirming the sensor integrity test has passed, reconnect the sensor.

Refer to [Alarms](#) for additional information.

Test Low and High Alarm Functions

6. **Low Alarm:** Apply a test gas concentration to the sensor. Ensure the gas concentration level is higher than the low alarm setpoint of the sensor.

The red LED flashes, **DANGER** displays and flashes on the LCD, and the audible alarm sounds (if enabled).

LOW ALARM displays below the sensor on the LCD that is in alarm. Audible, visual and/or relay alarms are engaged (if enabled).

7. **High Alarm:** Repeat the low alarm test procedures to test the high alarm.

System Inspection

Visually inspect the detector, all cables, option devices, and accessories. Ensure that the

- detector doors are securely closed,
- all port connections are securely connected, and
- outer weatherproof ring is fully screwed down.

Troubleshooting

If a problem occurs, refer to the solutions provided in Table 18. If a problem solution is not listed, calibrate the detector. If the problem cannot be resolved through calibration, contact [BW Technologies](#).

Table 18. Troubleshooting Tips

Problem	Possible Cause	Solution
If the LCD displays rF Out	Controller is deactivated	Activate the controller
	Antenna is not aligned	Move the antenna
	Radio Frequency (RF) signal from the controller is too weak	Move or replace the antenna Replace the antenna cable with low loss cable LMR 400. Refer to Replacement Parts and Accessories .
The signal is intermittent	Outside radio frequency interference (RFI)	Ensure all other radio equipment is grounded (e.g. base station)
The detector does not activate	Battery is drained	Charge the battery
	Battery is damaged or defective	Contact BW Technologies
	Main board fuse is blown	Contact BW Technologies Replace the main board assembly Contact BW Technologies
The LCD displays OFF	Measuring range set to zero	Match the gas cylinder measuring range to the measuring range of the encapsulated sensor/stainless sensor

Table 18. Troubleshooting Tips (cont.)

Problem	Possible Cause	Solution
There is a false alarm	Puff of target gas	System is functioning normally
	Not calibrated correctly	Check test gas and re-calibrate
There is no response to gas	Sensor is dirty	Clean or replace the sensor
	Expired or faulty sensor	Replace the sensor
There is radio frequency interference (RFI)	Incorrect bonding and grounding	Check grounding and bonding and remove interference
	Faulty or damaged sensor cable	Replace the cable
	Snow accumulation	Move the detector
The detector does not accurately measure gas	Sensor requires calibration	Calibrate the sensor
	Sensor screen is blocked	Clean sensor screen
The LCD is blank when the detector is activated	Main board fuse is blown	Contact BW Technologies
	Battery low (9.5 V)	Charge the battery
The LCD displays dCH ERR	Detector channel rotary switch is set to 0	Set the detector channel rotary switch to channel 1,2,3, or 4

Replacement Parts and Accessories

Warning

To prevent personal injury or damage to the detector, use only the specified replacement parts.

To order parts or accessories listed in the table below, contact [BW Technologies](#).

Table 19. Replacement Parts and Accessories

Model No	Description	Qty
Encapsulated Sensors / Caps / Filters		
SAII-L3H#	H ₂ S (hydrogen sulfide) encapsulated sensor	1
SAII-L3M1	CO (carbon monoxide) encapsulated sensor	1
SAII-L3X2	O ₂ (oxygen) encapsulated sensor	1
SAII-L3W1	% LEL (combustible) encapsulated sensor	1
SAII-L3S#	SO ₂ (sulfur dioxide) encapsulated sensor	1
SAII-L3A#	NH ₃ (ammonia) encapsulated sensor	1
SAII-L3C#	Cl ₂ (chlorine) encapsulated sensor	1
SAII-L3Y1	H ₂ (hydrogen) encapsulated sensor	1
SAII-L3Z1	HCN (hydrogen cyanide) encapsulated sensor	1
SAII-L3L2	HCl (hydrogen chloride) encapsulated sensor	1
SAII-L3D1	NO ₂ (nitrogen dioxide) encapsulated sensor	1
SAII-L3V1	ClO ₂ (chlorine dioxide) encapsulated sensor	1

Model No	Description	Qty
SAII-L3B2	C ₂ H ₅ OH (ethanol) encapsulated sensor	1
SAII-L3E1	C ₂ H ₄ O (ethylene oxide) encapsulated sensor	1
SAII-L3N2	NO (nitric oxide) encapsulated sensor	1
SAII-L3G1	O ₃ (ozone) encapsulated sensor	1
SAII-L3P1	PH ₃ (phosphine) encapsulated sensor	1
RRJ-FIL-K5	Sensor filters (encapsulated sensor)	5
M2493	Calibration cap for encapsulated sensor	1
Stainless Steel Sensors / Filters / Measuring Kits / Plugs		
PS-RH01	H ₂ S (hydrogen sulfide) sensor	1
PS-RX01	O ₂ (oxygen) sensor	1
PS-RM01	CO (carbon monoxide) sensor	1
PS-RS01	SO ₂ (sulfur dioxide) sensor	1
PS-RC01	Cl ₂ (chlorine) sensor	1
PS-RV01	ClO ₂ (chlorine dioxide)	1
PS-RA01	NH ₃ (ammonia) sensor	1
PS-RZ01	HCN (hydrogen cyanide) sensor	1
PS-RD01	NO ₂ (nitrogen dioxide) sensor	1
PS-RN01	NO (nitric oxide) sensor	1
PS-RL01	HCl (hydrogen chloride) sensor	1
PS-RB01	C ₂ H ₅ OH (ethanol) sensor	1
PS-RE01	C ₂ H ₄ O (ethylene oxide)	1
PS-RY01	H ₂ (hydrogen) sensor	1
PS-RG01	O ₃ (ozone) sensor	1

Model No	Description	Qty
PLxS-50-#-2K	Sensor measuring range change kit for stainless steel sensor units	1
MM-FIL-K2	Sensor filters (for toxic/O2)	
E0036	Calibration plug for stainless steel sensor assembly	
Cables and Connector Cable Interfaces		
UC2-S### (010 – 250)	Remote sensor cable	ft./ m
UC-PWR2-3-10	Dual power cables for solar panels	1
RR-EXT-UCxx (10-100)	Cable extension kit	1
RR-EXT-UC10	Cable extension kit (10ft./3m)	1
UC-SCAB2	24 Vdc direct operation connector cable interface (5 ft./1.5 m)	1
UC2-S010	Remote sensor cable with plug-in connectors (10 ft./3 m)	1
Antenna and Cable Assembly and Mounting Brackets		
RR-AN5	Antenna 5 dBi replacement	1
RR-AN8	Antenna 8 dBi with mounting bracket	1
RR-Acxx (10 or 20)	LMR 240 antenna cable assembly (ft./m)	1
RR-Acxxx (50 or 100)	LMR 400 antenna cable assembly (ft./m)	1
Chargers and Batteries		
UR-C300	Single bench charger 110 Vac with 5 ft./1.5 m cable	1

Model No	Description	Qty
UR-C404	Quad bench charger 110 Vac with 5 ft./1.5 m cable	
UR-S600	Weatherproof line trickle charger 110 Vac with 5 ft./1.5 m plug in cable	1
UR-TC10	Explosion proof link trickle charger 110 Vac with 5 ft./1.5 m plug in cable	1
Option Devices		
UR-L600	Strobe light with 60,000 candlepower	1
UR-LR60	Rechargeable strobe light with 160,000 candlepower	1
UR-H700	Siren alarm 101 dB	1
UR-HR70	Rechargeable siren alarm 101 dB	1
UR-HR60	Rechargeable bullhorn 112 dB	1
UR-LHR60	Rechargeable strobe/bullhorn with 160,000 candlepower and 112 dB	1
UR-J950	Multiple option box with 4 ports	1
Relays		
UD-RWS0	Single relay in weatherproof enclosure	1
UD-RWD0	Dual relay in weatherproof enclosure	1
UD-RES0	Single relay in explosion proof enclosure	1
UD-RED0	Dual relay in explosion proof enclosure	1
UD-RCS0	Single relay card with plug in cable (no enclosure)	1
UD-RCD0	Dual relay card with plug in cable (no enclosure)	1

Rig Rat III Detector

User Manual

Model No	Description	Qty
Security Accessories		
M1524	Security key	1
RR-LAT-1	Security latch (stainless steel)	1
Tripods and Wall Mounts Kits		
TRIPODx 1 or 2	Folding field tripod	1
TRI-EXT1	Tripod extension	1
TRI-PLATEx	Tripod option/accessory plate	1
MK-U600	Wall mounting kit	1
MK-EXT1	Extender sections for MK-U600	1
MK-PLATEx	Wall mount option plate	1
Datalogger/Cables/Software		
RS-DAT7-II	Datalogger	1
UA-DATC2	Datalogger RS232 port cable for RS-DAT7-II	1
UAII-DATS2	Software package with manuals and cable for RS-DAT7-II	1
Additional Replacement Parts and Accessories		
UAII-4-20MA	4-20MA interface for stand alone detectors	1
UA-ST24	Rechargeable solenoid driver 24 Vdc	1
RR-RTD-1	Transceiver assembly with bracket for detector	1
RR-FK-1	Fuse replacement 500 mA (set of 8)	1
E0216K	Replacement port cover caps 5-pin & 6-pin with chain, washer, and screws	1

Specifications

Instrument dimensions: 21.49 x 28.6 x 11.51 cm
(8.46 x 11.26 x 4.53 in.)

Weight: 5.15 kg (11 lbs. 6 oz.)

Enclosure: 14 gauge stainless steel NEMA/Type 4

Operating temperature: -40°C to +50°C (-40°F to +122°F)

Storage temperature: -40°C to +75°C (-40°F to +167°F)

Operating humidity: 5% to 95% relative humidity
(non-condensing)

Battery: 12 V, 3.4 amp hr. rechargeable battery

Battery operating time:

Charge life: Two toxic/oxygen sensors - 22 days
(without active trickle charge)

One toxic/oxygen sensor and one combustible sensor -
3 days (without active trickle charge)

RF frequency: 2.4 GHz frequency hopping spread spectrum
(FHSS)

RF transmission distance: 3 km (1.8 miles)

Alarm conditions: Low alarm, high alarm, loss of
transmission alarm, low battery alarm, and sensor integrity
alarm

Audible alarm: 85 dB at 1 m (3 ft.) oscillating

Visual alarm: Large red light-emitting diode (LED)

Security: Key lock access to control panel

Sensor heads: Plug-in, interchangeable, gas specific units

Sensor: Two 6-pin male ports

Supply voltage: Powered by the detector

Connector: 6-pin, MIL 5015 (14 S) female plug-in connector

Refer to [Appendix A Encapsulated Sensors](#) for operating specifications for each gas type

Combustible sensors: Poison-resistant catalytic bead

Current draw: 35 mA typical at 12 Vdc

Output signal: 0 to -500 millivolt signal at option port

Enclosure: Encapsulated duraprene

Size (l x w x h): 6.90 x 8.20 x 5.79 cm (2.72 x 3.23 x 2.28 in.)

Weight: 175 g (6.2 oz.)

Approved: Class I, Div. 1, Groups C, D; Class II, Div. 1, Group G

Toxic/Oxygen sensors: Electrochemical cells

Current draw: 4 mA maximum at 12 Vdc

Output signal: 0 to -500 millivolt signal at option port

Enclosure: Encapsulated duraprene

Size (l x w x h): 6.90 x 8.20 x 5.79 cm (2.72 x 3.23 x 2.28 in.)

Weight: 175 g (6.2 oz.)

Approved: Class I, Div. 1, Groups C, D; Class II, Div. 1, Group G

Display: Alphanumeric liquid crystal display (LCD)

Calibration: Automatic zero and automatic span

User field options: Maximum gas level, transmission test, sensor disable, loss of transmission time interval, transmitter disable

Connections: Plug-in, mil-style, amphenol connectors with weatherproof covers

Sensor: Two 6-pin male ports

Charger: One 5-pin female port

Options: Two 6-pin female ports

Antenna: One port with TNC connector

Normal charge: 1 hour per battery

Intrinsic Safety: Approved by CSA to both U.S. and Canadian standards

Approved: Class I, Division 1, Group C and D, T3C; Class 2, Group G, T3C

Standards: CAN/CSA C22.2 No. 157 and C22.2 152
ANSI/UL – 913 and ANSI/ISA – S12.13 Part 1

Appendix A Encapsulated Sensors

<u>Sensor Specifications (Encapsulated)</u>	57
<u>Calibration Gas Specifications</u>	60
<u>Encapsulated Sensor Measuring Ranges</u>	61
<u>Relative Sensitivity of Combustible Gases/Vapors</u>	62

Sensor Specifications (Encapsulated)

Table 20. Operating and Calibration Specifications for Each Encapsulated Sensor

Specifications	Combustibles %LEL	Oxygen O ₂ % by vol.	Hydrogen Sulfide H ₂ S ppm	Sulfur Dioxide SO ₂ ppm	Carbon Monoxide CO ppm	Ammonia NH ₃ ppm
Repeatability % of signal	1	0.1	1	1	1	10
Operating temperature range °C °F	-40 to +50 -40 to +122	-20 to +50 -4 to +122	-40 to +50 -40 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +40 -4 to +104
Operating humidity	5 to 95% non-condensing					
Long term drift Zero: % of signal loss/month Span:	Nominal <1 %	Nominal <1 % ¹	Nominal <2	Nominal <2	Nominal <2	Nominal <2
LCD increments	1%	0.1%	1 ppm	1 ppm	1 ppm	1 ppm
Calibration	250	250	250	400	150	250
Flow rate ml/min. at a % or ppm reading of:	25%	20.9%	50 ppm	20 ppm	200 ppm	50 ppm

¹ For <1 %1: Oxygen sensor drift is <5% over operating life.

Table 20. Operating and Calibration Specifications for Each Encapsulated Sensor

Specifications	Chlorine Cl ₂ ppm	Hydrogen H ₂ ppm	Hydrogen Cyanide HCN ppm	Hydrogen Chloride HCl ppm	Nitrogen Dioxide NO ₂ ppm	Chlorine Dioxide ClO ₂ ppm
Repeatability % of signal	2	2	2	2	2	2
Operating temperature range °C °F	-20 to +40 -4 to +104	-20 to +50 -4 to +122	-40 to +40 -40 to +104	-20 to +40 -4 to +104	-20 to +50 -4 to +122	-20 to +40 -4 to +104
Operating humidity	5 to 95% non-condensing					
Long term drift Zero:	Nominal	Nominal	Nominal	Nominal	Nominal	Nominal
% of signal loss/month Span:	<2	<2	<5	<3	<2	<2
LCD increments	0.1 ppm	1 ppm	0.01 ppm	0.1 ppm	0.1 ppm	0.1 ppm
Calibration	1000	150	400	1000	400	1000
Flow rate ml/min. at a % or ppm reading of:	2 ppm	100 ppm	15 ppm	15 ppm	10 ppm	5 ppm

Table 20. Operating and Calibration Specifications for Each Encapsulated Sensor

Specifications	Ethanol C ₂ H ₅ OH ppm	Ethylene Oxide C ₂ H ₄ O ppm	Nitric Oxide NO ppm	Ozone O ₃ ppm	Phosphine PH ₃ ppm	Phosgene COCl ₂ ppm
Repeatability % of signal	1	1	2	5	2	2
Operating temperature range °C °F	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +40 -4 to +104	-20 to +50 -4 to +122	-20 to +40 -4 to +104
Operating humidity	15 to 90% non-condensing					
Long term drift Zero: % of signal loss/month Span:	Nominal <2	Nominal <2	Nominal <2	Nominal <2	Nominal <2	Nominal <5
LCD increments	1 ppm	1 ppm	1 ppm	0.1 ppm	0.1 ppm	0.1 ppm
Calibration Flow rate ml/min. at a % or ppm reading of:	1000 ² 10 ppm	1000 10 ppm	400 50 ppm	1000 0.8 ppm	1000 1 ppm	1000 0.3 ppm

² For 1000: To calibrate ethanol use 10 ppm of ethylene oxide.

Note: Performance data is based upon conditions at 20°C, 50% RH, 1013 mBar.

Calibration Gas Specifications

Toxic and Oxygen: Electrochemical

Combustible: Catalytic

Position sensitivity: None

Operation pressure range: 900 to 1100 mBar (Atmospheric +/- 10%)

Calibration notes: For maximum accuracy, calibrate with a mixture in the range most measurements will be made. For most purposes, a 2 minute exposure is satisfactory.

Remote calibration: Allow a longer period of time when applying gas, dependent upon the length of the hose.

Calibration hose: Use Teflon, Tygon, or stainless steel hose on all sensors.

Caution

Tygon will poison a combustible sensor over time.

Combustible sensor: For the most accurate measurements calibrate using the gas or vapor under investigation. Where this is not possible, refer to Table 22 Relative Sensitivity.

Measuring Ranges for Encapsulated Sensors

Table 21. Encapsulated Sensor Measuring Ranges

Gas Type	Sensor Part #	Units of Measure	Measuring Ranges Available					
			When ordering, substitute # in the part number for the number located at the top of the column					
			1	2	3	4	5	6
LEL (Combustibles)	SAII-L3W1	% LEL	0 to 100					
O ₂ (Oxygen)	SAII-L3X#	% by vol.	0 to 25.0	0 to 30.0				
H ₂ S (Hydrogen sulfide)	SAII-L3H#	ppm	0 to 100	0 to 50	0 to 500	0 to 20		
SO ₂ (Sulfur dioxide)	SAII-L3S#	ppm	0 to 100		0 to 20	0 to 10		
CO (Carbon monoxide)	SAII-L3M1	ppm	0 to 500					
NH ₃ (Ammonia)	SAII-L3A#	ppm	0 to 50	0 to 100				
Cl ₂ (Chlorine)	SAII-L3C#	ppm	0 to 5.0			0 to 10.0		
H ₂ (Hydrogen)	SAII-L3Y#	ppm	0 to 100					0 to 500
HCl (Hydrogen chloride)	SAII-L3L2	ppm				0 to 20.0		
HCN (Hydrogen cyanide)	SAII-L3Z1	ppm	0 to 20.0					
NO ₂ (Nitrogen dioxide)	SAII-L3D1	ppm	0 to 10.0					
ClO ₂ (Chlorine dioxide)	SAII-L3V1	ppm	0 to 5.0					
C ₂ H ₅ OH (Ethanol)	SAII-L3B2	ppm					0 to 1000	
C ₂ H ₄ O (Ethylene oxide)	SAII-L3E1	ppm	0 to 10.0					
NO (Nitric oxide)	SAII-L3N2	ppm					0 to 100.0	
O ₃ (Ozone)	SAII-L3G1	ppm	0 to 1.0					
PH ₃ (Phosphine)	SAII-L3P1	ppm	0 to 10.0					

Relative Sensitivity of Combustible Gases/Vapours

The following table shows the variation of the combustible sensor when exposed to a range of gases and vapors at the same % LEL concentration. The figures are expressed relative to the methane signal (=100).

The results are intended for guidance only. For a more accurate measurement, calibrate using the gas or vapor under investigation.

Table 22. Relative Sensitivity of Combustible Gases/Vapours

Gas/Vapor	Relative Sensitivity	Gas/Vapor	Relative Sensitivity
Methane	100	Carbon monoxide	110
Propane	65	Acetone	75
n-Butane	60	Methyl ethyl ketone	60
n-Pentane	50	Toluene	60
n-Hexane	50	Ethyl acetate	65
n-Heptane	50	Hydrogen	100
n-Octane	50	Ammonia	145
Methanol	115	Cyclohexane	65
Ethanol	85	Leaded petrol	60
iso-Propyl Alcohol	70	Unleaded petrol	60


Note: Each sensitivity has been rounded to the nearest 5%.

Appendix B Installation Requirements

<u>Installation of an Unapproved Charger – Detector</u>	64
<u>Detector System Interconnection</u>	64
<u>List 1</u>	65
<u>Installation of an Unapproved External Charger</u>	66
<u>Barrier Parameters</u>	68
<u>IS Sensor Barrier</u>	72

Installation of an Unapproved Charger — Detector**Detector System Interconnection**

Note: The diagram below shows the cable limitations and regulations for connecting to detector ports in Class I, Div 1 areas. Violations of these parameters will impair Intrinsic Safety.

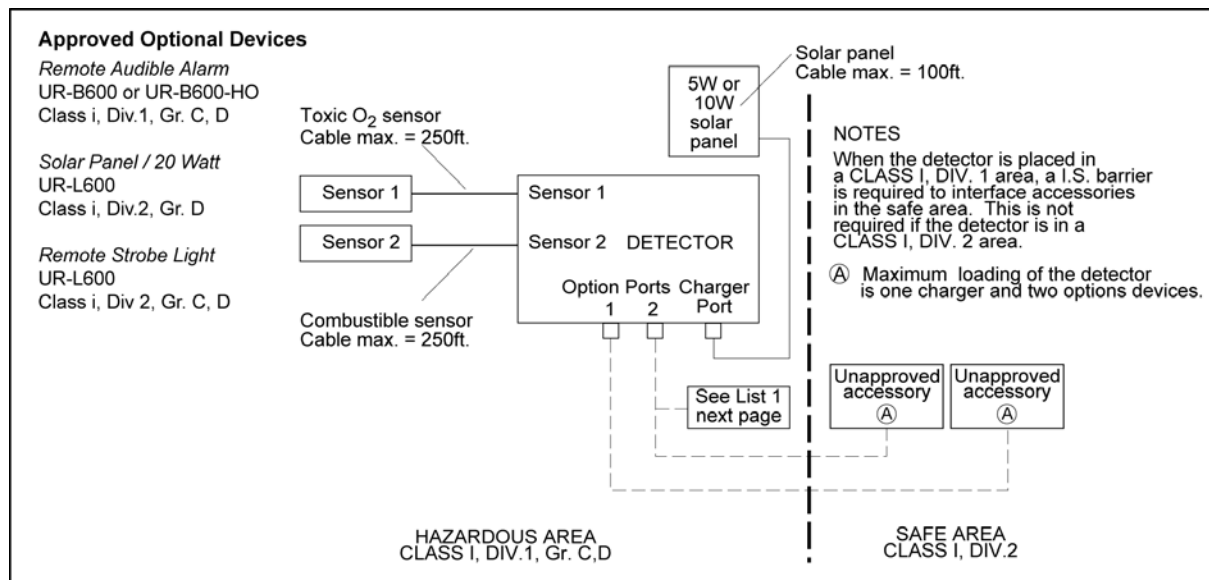**Figure 24. Gas Detection System Interconnection**

List 1

Approved Class I, Div. 1, Gr. C, D Alarms

- UR-B600

Approved Class I, Div. 2, Gr. C, D Alarms

- UR-L600
- UR-L601
- UR-L602

Table 23. Limiting Energy

I.S. Barrier		Detector
Open circuit voltage, VOC	≤	Vmax, maximum voltage allowed
Short circuit current, Isc	≤	Imax, maximum current allowed
Allowed capacitance, Ca	≥	Ci, internal capacitance +Ccable, cable capacitance
Allowed inductance, La	≥	Li, internal inductance +Lcable, cable inductance
Ca and La include capacitance and inductance		

Installation of an Unapproved External Charger

Note: When the sensor and detector are in a Class I, Div. 2, Gr. C, D hazardous area and an unapproved external charger is installed in a safe area, barriers are not required.

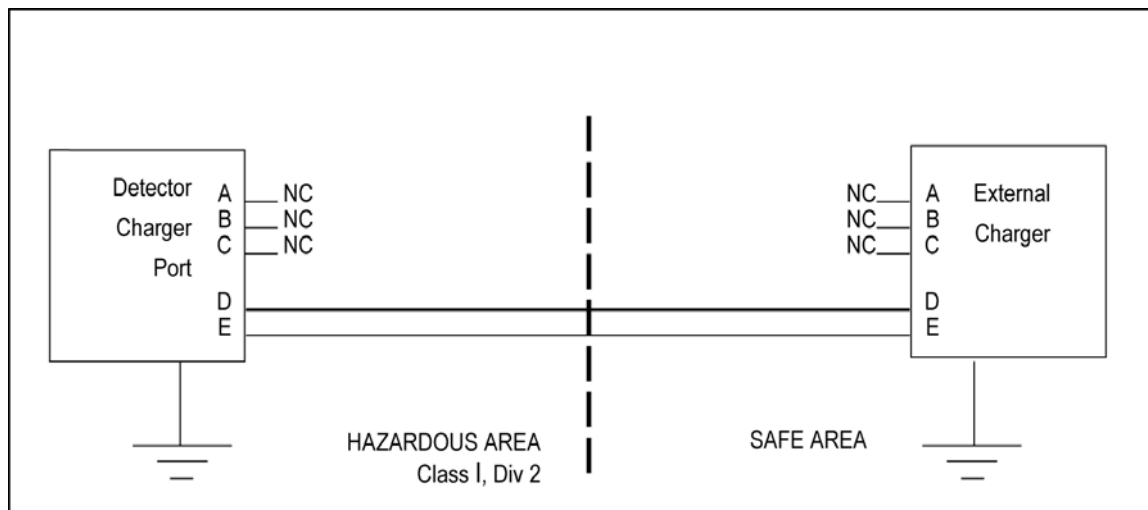


Figure 25. Division 2 Unapproved External Charger Installation

Note: When installing an unapproved external charger in a Class I, Div. 1, Gr. C, D hazardous area, install barriers as shown in Figure 26 to ensure Intrinsic Safety.

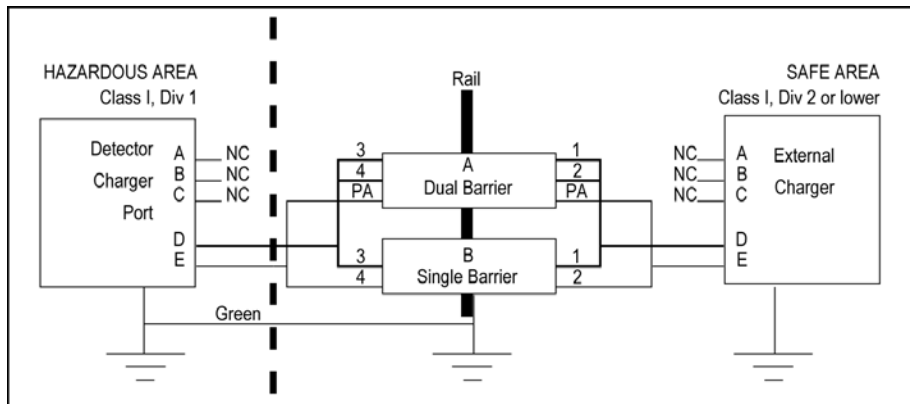


Figure 26. Division 1 Unapproved External Charger Installation

Requirements:

1. This configuration is required for the charger port.
2. I.S. barriers required for Class I, Div. 1 applications only.
3. All intrinsically safe wiring shall be kept separate from non-intrinsically safe wiring.
4. Use Beldon SJTW3 cable or the equivalent.

Note: Any barrier that meets the entity parameter criteria is acceptable.

Barrier Parameters

Voc Isc Ca La

19.9 V 150 mA 1.00uF 7.0 mH

Table 24. I.S. Barrier Example

Barrier	Example - Dual	
	Qty	STAHL P/N
A	1	9002/77-220-296-00
B	1	9001/01-199-150-10

The installation must comply with the Canadian Electrical Code (CEC) and the National Electrical Code (NEC).

Note: When the sensor and detector are in a Class I, Div. 2, Gr. C, D hazardous area and an unapproved accessory is installed in a safe area, barriers are not required.



Figure 27. Division 2 Unapproved Accessory Installation

Note: When installing an unapproved accessory in a Class I, Div. 1, Gr. C, D hazardous area, install barriers as shown in the following figure to ensure Intrinsic Safety.

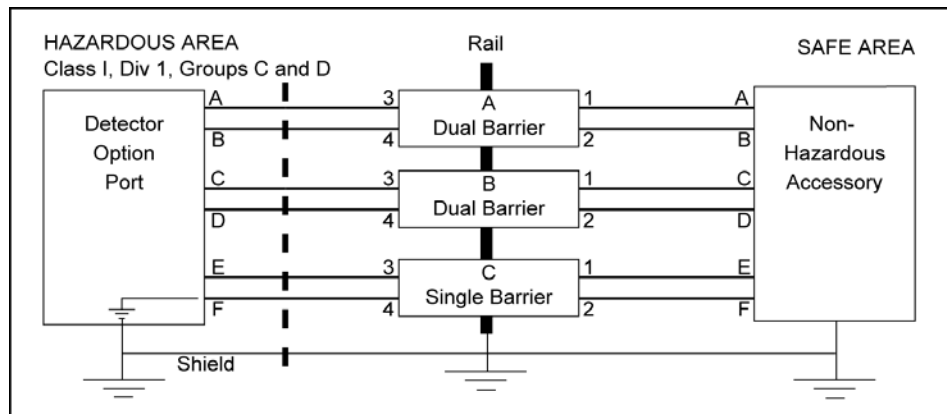


Figure 28. Division 1 Unapproved Accessory Installation

Requirements:

1. This configuration is required for each option port.
2. I.S. barriers required for Class I, Div. 1 applications only.
3. All intrinsic safe wiring shall be kept separate from non-intrinsically safe wiring.
4. Electrical Parameters of the cable: capacitance = 60pF/ft. and inductance = 0.20 uH/ft. where $C_a > C_i + C_{\text{cable}}$ and $L_a > L_i + L_{\text{cable}}$.

Table 25. I.S. Barrier Configurations

Terminal	Voc	Isc	Ca	La
A Reference > to ground	15 V	150 mA	1.2 uF	4.5 mH
B Reference > to ground	15 V	150 mA	1.2 uF	4.5 mH
C Reference > to ground	8.2 V	150 mA	10.8 uF	4.2 mH
D Reference > to ground	8.2 V	150 mA	10.8 uF	4.2 mH
E Reference > to ground	15 V	390 mA	1.2 uF	0.54 mH

Any barrier that meets the entity parameter criteria is acceptable. The following table provides some possible choices.

Table 26. I.S. Barrier Requirements

Barrier	Option 1 - Dual	
	Qty	STAHL P/N
A	1	9002/77-150-300-00
B	1	9002/22-093-300-00
C	1	9001/01-158-390-10 (Single barrier)

The installation must comply with the Canadian Electrical Code (CEC) and the National Electrical Code (NEC).

IS Sensor Barrier Installation

Note: The following figure outlines the installation of a sensor in a hazardous area using the IS Sensor Barrier. The IS barrier is approved for installation in Group B or C.

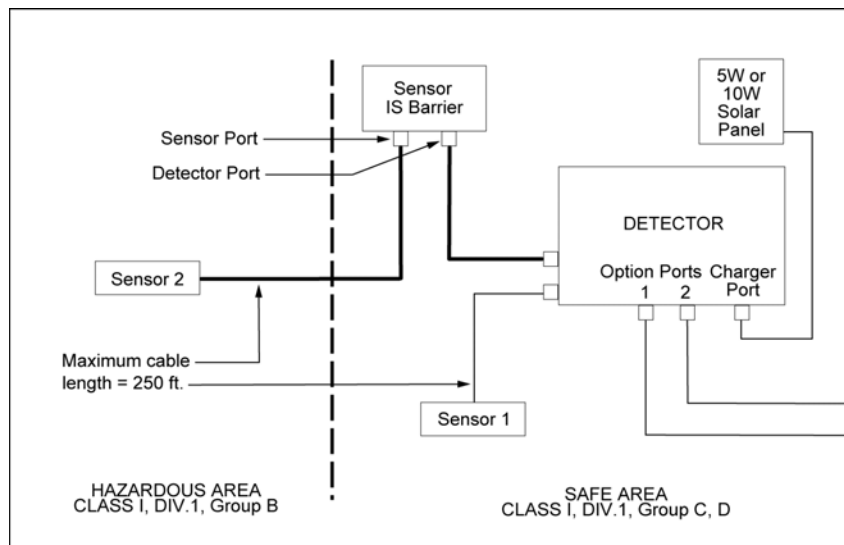


Figure 29. Approved IS Sensor Barrier Installation

For information and requirements about installing option accessories in a hazardous area, refer to [Detector System Interconnection](#) and Figure 25 Gas Detection System Interconnection.

Appendix C Stainless Steel Sensors

Stainless Steel Sensors Toxic/O₂	74
Installation	74
Calibration (Stainless Steel Sensors)	74
Auto Zero	74
Cylinder Connection and Sensor Installation	75
Span the Sensors and Detector	75
Transmission Interval	77
Loss of Transmission Time Interval	78
End Calibration	79
Maintenance	79
Replace Toxic/O₂ Sensor Cells and Screen	80
Specifications (Stainless Steel Sensors)	81
Sensor Measuring Ranges (Stainless Steel)	85

Stainless Steel Sensors (Toxic/O₂)

Installation

For proper installation of the toxic/O₂ stainless steel sensor, please refer to the following figure.

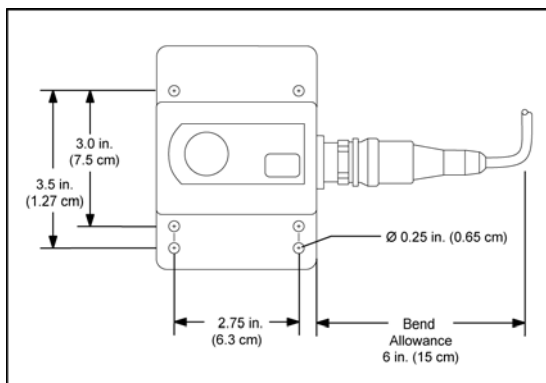


Figure 30. Sensor Dimensions (Stainless Steel)

Calibration (Stainless Steel Sensors)


Auto Zero

⚠ Caution

Perform the following calibration procedures in a clean atmosphere that is free of hazardous gas, otherwise connect a zero gas cylinder.

To set the setpoint to 0 (zero), complete the following:

8. From the operations bay panel, press ☐ LOW/▼ or ☐ HIGH/▲ until **0** (zero) displays on the detector LCD.

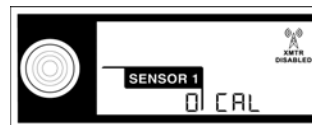

9. Press ☐ OK to accept the new value.

Note

Zero drift for the O₂ sensor is extremely minimal over the life span of the sensor. If zeroing is required, apply 100% Nitrogen (N₂).

Cylinder Connection and Installation

10. Insert the calibration cap into the stainless steel sensor as shown in Figure 31.


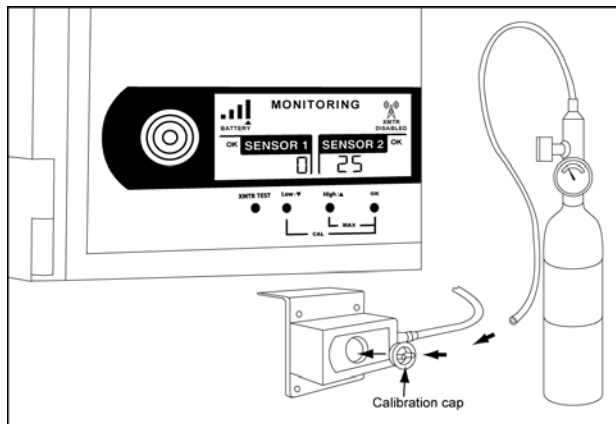


Figure 31. Cylinder Connection for Calibration

11. Connect the hose to the cylinder. Do not attach the hose to the sensor until instructed to apply gas.

Span the Sensors and Detector

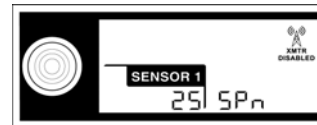

Note

Using 50% LEL gas is recommended.

12. Connect the hose to the calibration cap and open the valve on the cylinder. Apply gas to the sensor until the LCD readout stabilizes (approximately 2 minutes).
13. To adjust the current value on the detector, press ☐ LOW/▼ or ☐ HIGH/▲ until the required value displays.
14. Press ☐ OK to accept the new value.
15. Remove the gas from the sensor and close the valve of the gas cylinder. Allow the detector time to display a zero reading.

Detector Does Not Return to Zero Reading: If the sensor reading does not return to zero, ensure that the sensor measuring range rotary switch is set correctly.

Reset the rotary switch if required and repeat the calibration procedures. Repeat the calibration procedures for SENSOR 2 (if applicable) before setting the transmission interval in the following section

Transmission Interval

Note

Before proceeding, ensure that both SENSOR 1 and SENSOR 2 (if applicable) have been calibrated.

The transmission interval is used to set the detector to transmit data to the controller on a regularly scheduled basis. The detector can be set to transmit data once a day, hourly, or more frequently.

- Minimum 5 seconds
- Maximum 25 hours

To set/change the transmission time, complete the following:

16. Determine how frequently the transmissions are to be sent to the controller.

Note

Frequent transmissions require that the battery be recharged more frequently.

17. From the detector, press ☐ LOW/▼ and ☐ OK simultaneously to enter calibration mode (if required).
18. From calibration mode, press ☐ LOW/▼ and ☐ OK simultaneously again to access the transmission time screen.

The hours **00h** interval screen initially displays.



19. Press ☐ LOW/▼ or ☐ HIGH/▲ until the required hour(s) value displays (maximum 25 hours).
20. Press ☐ OK to accept the new value.

Or


For more frequent transmissions (less than 1 hour), press ☐ OK to bypass and automatically access the minutes **00.** interval screen.



21. Press ☐ LOW/▼ or ☐ HIGH/▲ until the required minute(s) value displays.
22. Press ☐ OK to accept the new value.

Or

For more frequent transmissions (less than 1 minute), press ☐ OK to bypass and automatically access the seconds **.00 int** screen.

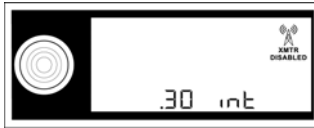

23. Press ☐ LOW/▼ or ☐ HIGH/▲ until the required seconds value displays (minimum .05 seconds).
24. Press ☐ OK to accept the new value.

The loss of transmission time interval screen **00h t.E** displays.

Loss of Transmission Time Interval



In the event that transmissions are interrupted, this function is used to enter a specified time that a controller will wait for transmissions from a detector before entering an alarm state.


- Maximum period of standby: 97 hours
- Minimum period of standby: 1 minute

To enter a loss of transmission time interval, complete the following:

25. The initial loss of transmission time interval (**00h t.E**) screen displays the hours (**00h**). Press ☐ LOW/▼ or ☐ HIGH/▲ until the desired hour(s) value displays.
26. Press ☐ OK to accept the new value.

Or


For reduced transmission time interval (less than 1 hour), press ☐ OK to bypass and automatically access the minutes (**00. t.E**) screen.

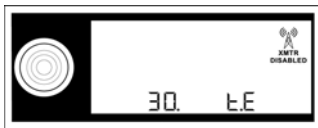

27. Press ☐ LOW/▼ or ☐ HIGH/▲ until the desired minute(s) value displays.
28. Press ☐ OK to accept the new value.

The end calibration screen displays.

End Calibration

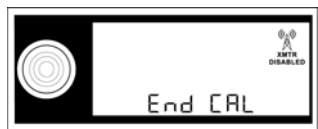

After the loss of transmission time interval is set, the LCD displays **End CAL** to signal the end of the calibration procedure.

Maintenance

The toxic/O₂ sensor is equipped with two washable screens for added protection against damage. If the screen becomes dirty or blocked, clean with a soft brush, mild soap, and water.

Ensure that the sensor blanking plugs and calibration cap is inserted when the detector is deactivated and in transit (refer to figure 32). The blanking plugs can be used to protect the sensor from paint and solvent fumes.

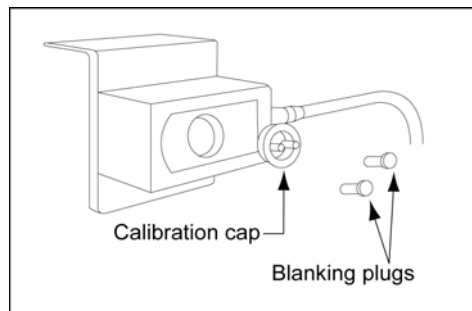


Figure 32. Calibration Cap and Blanking Plugs

If a sensor screen is damaged or punctured, replace it immediately.

Replace Toxic/O₂ Sensor Cells and Screen

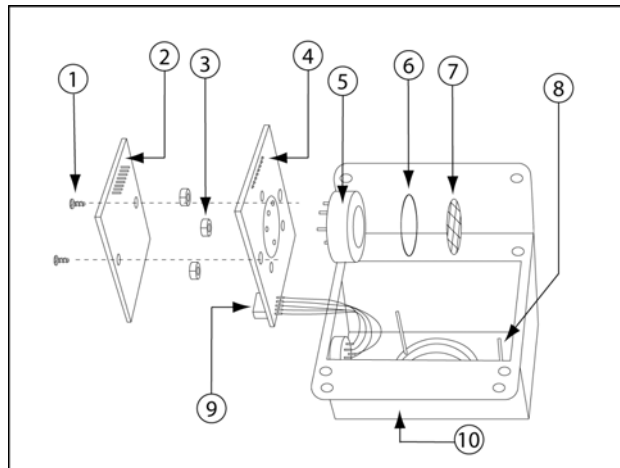


Figure 33. Toxic/O₂ Sensor Replacement

1. Using a Phillips screwdriver, remove the four screws on the back cover to open the sensor head.
2. Remove the two screws that hold the measuring range module onto the main board.

Table 27. Toxic/O₂ Sensor Replacement Parts

Item	Description
1	Phillips screws for measuring range module
2	Measuring range module with 8-pin header
3	Hex screws
4	Main board with 8-pin terminal block
5	Sensor
6	O-ring
7	Sensor screen
8	Screws
9	Harness
10	Sensor head

3. Gently remove the module from the 8-pin terminal block.
4. Using a 5/32" hex driver, remove the three hex screws that attach the main board. Unplug the harness and remove the board.

5. **Screen replacement:** Replace the sensor screen.
Sensor replacement: Remove the old sensor and insert the new sensor onto the board.
6. Ensure that the sensor screen and O-ring are assembled in the correct order.
7. Replace the main board, the three hex screws, insert in the harness, and replace the measuring range module. Ensure the module gas matches the sensor.
8. Replace the back enclosure, washers, and screws.
9. Calibrate the sensor.

Specifications (Stainless Steel Sensors)

Toxic/Oxygen sensor: Electrochemical cells

Current draw: 2 mA maximum at 12 V dc

Output signal: 0 to -500 millivolt signal at option port

Sensor screens: Two washable PTFE (Teflon) mesh

Enclosure: 16-gauge stainless steel, NEMA 3R, RFI/EMI shielded

Size (l x w x h): 11.5 x 9.1 x 8.0 cm (4.5 x 3.5 x 3.1 in.)

Weight: 0.8 kg (1.9 lbs.)

Approved: Class I, Div. 1, Groups C, D; Class II, Div. 1, Group G

Table 28. Operating and Calibration Specifications for Each Stainless Steel Sensor

Specifications	Combustibles %LEL	Oxygen O ₂ % by vol.	Hydrogen Sulfide H ₂ S ppm	Sulfur Dioxide SO ₂ ppm	Carbon Monoxide CO ppm
Repeatability % of signal	1	0.1	1	1	1
Operating temperature range °C °F	-40 to +50 -40 to +122	-20 to +50 -4 to +122	-40 to +50 -40 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122
Operating humidity	5 to 95% non-condensing				
Long term drift Zero: % of signal loss/month Span:	Nominal <1 %	Nominal <1 % ¹	Nominal <2	Nominal <2	Nominal <2
LCD increments	1%	0.1%	1 ppm	1 ppm	1 ppm
Calibration	250	250	250	400	150
Flow rate ml/min. at a % or ppm reading of:	25%	100% N ₂	20 ppm	20 ppm	200 ppm

1: O₂ sensor drift is <5% over operating life.

Table 28. Operating and Calibration Specifications for Each Stainless Steel Sensor (cont.)

Specifications	Ammonia NH₃ ppm	Chlorine Cl₂ ppm	Hydrogen H₂ ppm	Hydrogen Cyanide HCN ppm	Hydrogen Chloride HCl ppm	Nitrogen Dioxide NO₂ ppm
Repeatability % of signal	10	2	2	2	2	2
Operating temperature range °C °F	-25 to +35 -13 to +95	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122
Operating humidity	5 to 95% non-condensing					
Long term drift Zero: % of signal loss/month Span:	Nominal <2	Nominal <2	Nominal <2	Nominal <2	Nominal <2	Nominal <2
LCD increments	1 ppm	0.1 ppm	1 ppm	0.01 ppm	0.1 ppm	0.1 ppm
Calibration Flow rate ml/min. at a % or ppm reading of:	250 25 ppm	1000 10 ppm	150 10 ppm	400 10 ppm	1000 20 ppm	400 10 ppm

Table 28. Operating and Calibration Specifications for Each Stainless Steel Sensor (cont.)




Specifications	Chlorine Dioxide ClO ₂ ppm	Ethanol C ₂ H ₅ OH ppm	Ethylene Oxide C ₂ H ₄ O ppm	Nitric Oxide NO ppm	Ozone O ₃ ppm
Repeatability % of signal	2	1	1	2	5
Operating temperature range °C °F	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122	-20 to +50 -4 to +122
Operating humidity	5 to 95% non-condensing	15 to 90% non-condensing			
Long term drift Zero: % of signal loss/month Span:	Nominal <2	Nominal <5	Nominal <5	Nominal <2	Nominal <2
LCD increments	0.1 ppm	1 ppm	1 ppm	1 ppm	0.01 ppm
Calibration Flow rate ml/min. at a % or ppm reading of:	1000 10 ppm	1000 20 ppm	1000 20 ppm	400 10 ppm	1000 1 ppm

Note: Performance data is based on conditions at 20°C, 50% RH, 1013 mBar.

Measuring Ranges for Stainless Steel Sensors

Table 29. Stainless Steel Sensor Measuring Ranges

Gas Type	Sensor Part #	Units of Measure	Measuring Ranges Available							
			When ordering, substitute # in the part number for the number located at the top of the column						Sensor Cell #	Sensor Range Module Part#
			1	2	3	4	5	6		
LEL (Combustibles)	SA11-L3W1	% LEL	0 - 100						E2333	PLWS-50-#
O ₂ (Oxygen)	SA-L2X1	% by vol.	0 - 25.0	0 - 30.0					PS-RX01	PLXS-50-#
H ₂ S (Hydrogen sulfide)	SA-L2H#	ppm	0 - 100	0 - 50	0 - 500	0 - 20	0 - 30		PS-RH01	PLHS-50-#
SO ₂ (Sulfur dioxide)	SA-L2S#	ppm	0 - 100	0 - 50	0 - 20	0 - 10			PS-RS01	PLSS-50-#
CO (Carbon monoxide)	SA-L2M1	ppm	0 - 500	0 - 1000	0 - 100	0 - 50	0 - 200	0 - 600	PS-RM01	PLMS-50-#
NH ₃ (Ammonia)	SA-L2A#	ppm	0 - 50	0 - 100			0 - 150		PS-RA01	PLAS-50-#
Cl ₂ (Chlorine)	SA-L2V#	ppm	0 - 5.0	0 - 10.0	0 - 250				PS-RV01	PLCS-50-#
H ₂ (Hydrogen)	SA-L2Y#	ppm	0 - 100	0 - 200	0 - 800				PS-RY01	PLYS-50-#
HCl (Hydrogen chloride)	SA-L2L#	ppm	0 - 10.0	0 - 20.0	0 - 100				PS-RL01	PLLS-50-#
HCN (Hydrogen cyanide)	SA-L2Z#	ppm	0 - 20.0	0 - 50.0	0 - 100				PS-RZ01	PLZS-50-#
NO ₂ (Nitrogen dioxide)	SA-L2D#	ppm	0 - 10.0	0 - 20.0					PS-RD01	PLDS-50-#
ClO ₂ (Chlorine dioxide)	SA-L2V	ppm		0 - 1.0					PS-RV01	PLVS-50-#
C ₂ H ₅ OH (Ethanol)	SA-L2B	ppm	0 - 500						PS-RB01	PLBS-50-#
C ₂ H ₄ O (Ethylene oxide)	SA-L2E	ppm	0 - 10.0	0 - 20.0					PS-RE01	PLES-50-#
NO (Nitric oxide)	SA-L2N	ppm	0 - 50.0						PS-RN01	PLNS-50-#
O ₃ (Ozone)	SA-L2G	ppm	0 - 1.0	0 - 2.0					PS-RG01	PLGS-50-#





D2124/3 English

iERP: 118434

© 2005 BW Technologies, all rights reserved. Printed in Canada.

All product names are trademarks of their respective companies.



3 3/4 in.	 Corporate Headquarters Calgary, Alberta Technologies <small>by Honeywell</small>	ERRATA CARD	123703 Rig Rat III Controller & Rig Rat III Detector
	<p>The following information has changed for: Rig Rat III Controller User Manual (D2135/1) RigRat III Detector User Manual (D2124/3)</p> <p>Specifications</p> <p>This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules and ICES-003 Canadian EMI requirements. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:</p> <ul style="list-style-type: none"> • Reorient or relocate the receiving antenna. • Increase the separation between the equipment and receiver. 	<ul style="list-style-type: none"> • Connect the equipment into an outlet on a circuit different from that to which the receiver is connected. • Consult the dealer or an experienced radio/TV technician for help. <p>The following information has changed for: Rig Rat III Controller User Manual (D2135/1)</p> <p>BW Europe 5 Canada Close Banbury, Oxfordshire UK OX16 2RT</p> <p>Contacting BW Technologies</p> <p>Europe: +44 (0) 1295 700300</p>	
<div style="text-align: center;">5 1/2 in.</div>			

Printing Information

iERP #	123703
Size:	3 3/4 x 5 1/2 inches
Stock:	80 lb cougar cover card stock
Print Color:	Black
Language:	English